

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070820\
 Data File : FE032319.D
 Signal(s) : FID1B.CH
 Acq On : 08 Jul 2020 16:21
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 09 01:03:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE070720.M
 Quant Title :
 QLast Update : Wed Jul 08 12:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.748	16372975	53.820 ug/ml
Target Compounds			
2) N-DECANE	4.493	18779346	53.999 ug/ml
3) N-DODECANE	6.509	18863730	54.054 ug/ml
4) N-TETRADECANE	8.303	18850002	54.243 ug/ml
5) N-HEXADECANE	9.905	18931800	54.301 ug/ml
6) N-OCTADECANE	11.346	19194370	54.279 ug/ml
7) N-EICOSANE	12.655	19035339	54.124 ug/ml
8) N-DOCOSANE	13.853	18954465	53.942 ug/ml
10) N-TETRACOSANE	14.954	19007965	53.698 ug/ml
11) N-HEXACOSANE	15.974	18741969	53.409 ug/ml
12) N-OCTACOSANE	16.922	18691757	53.147 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070820\
Data File : FE032319.D
Signal(s) : FID1B.CH
Acq On : 08 Jul 2020 16:21
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 09 01:03:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE070720.M
Quant Title :
QLast Update : Wed Jul 08 12:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

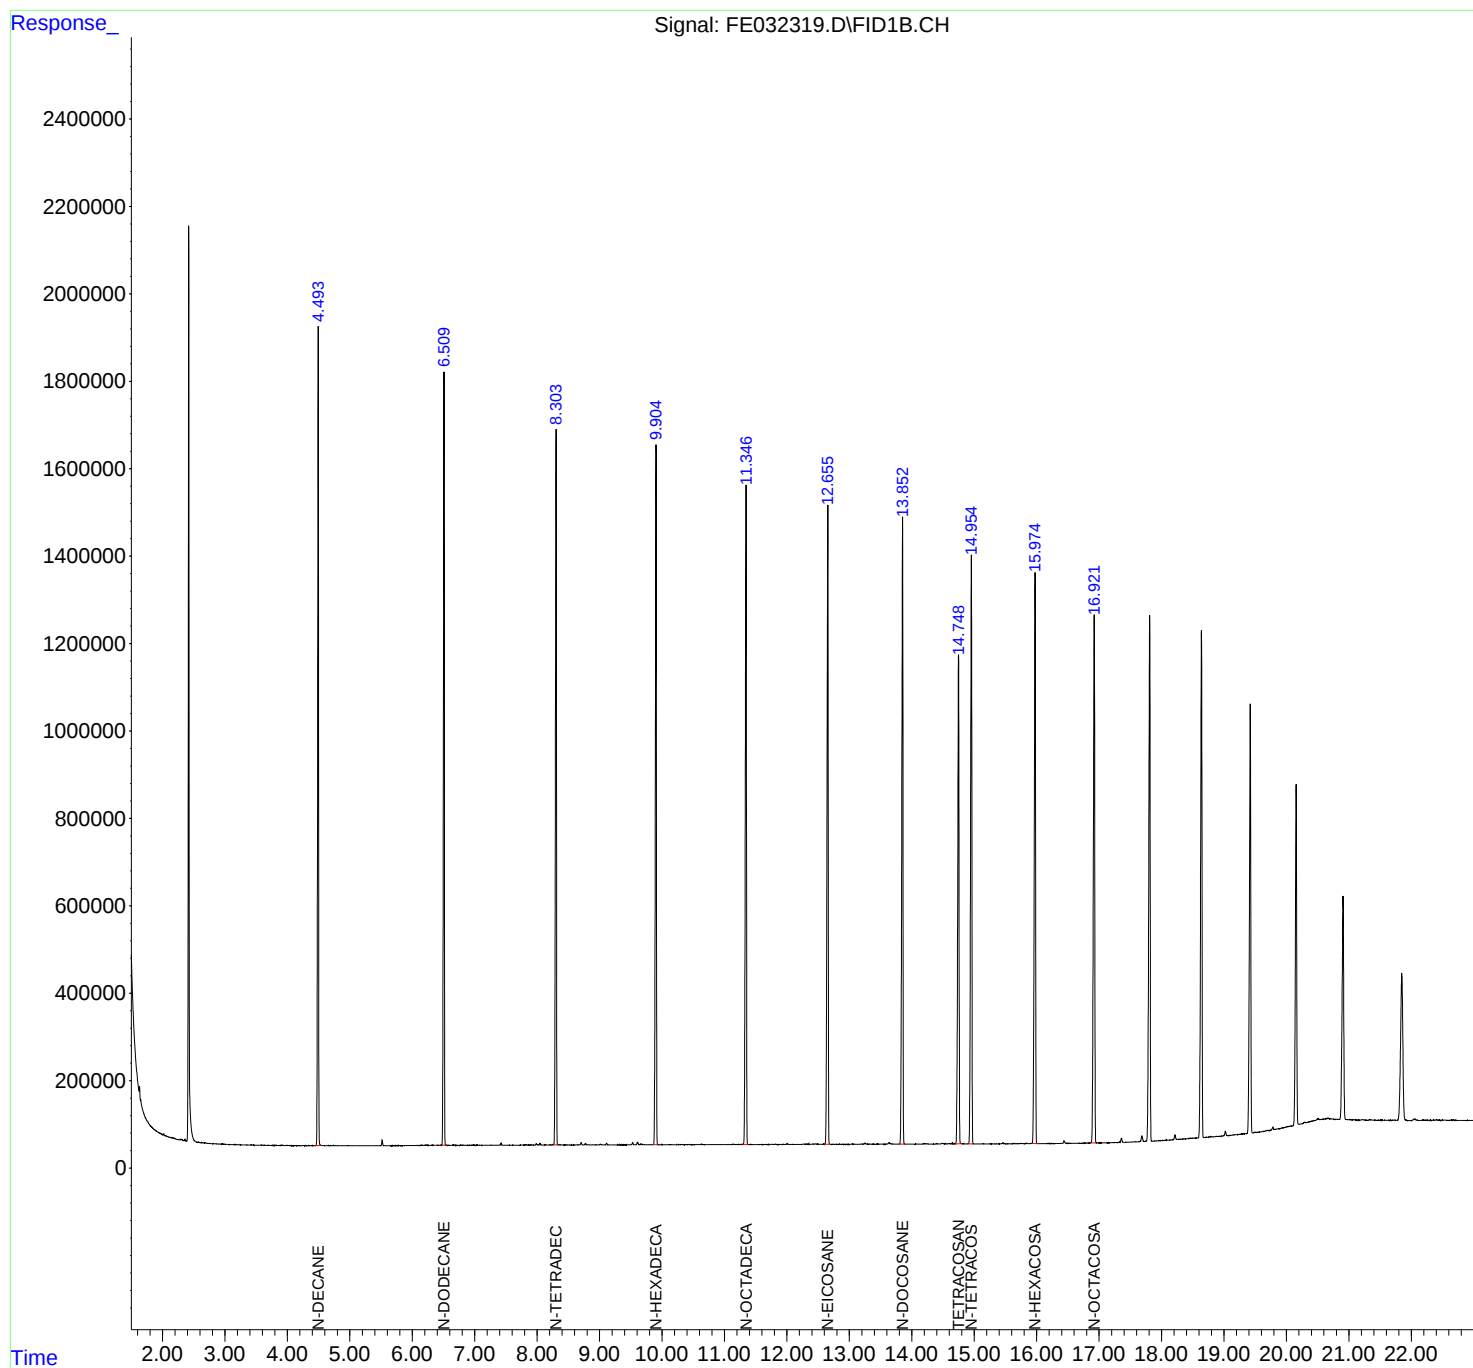

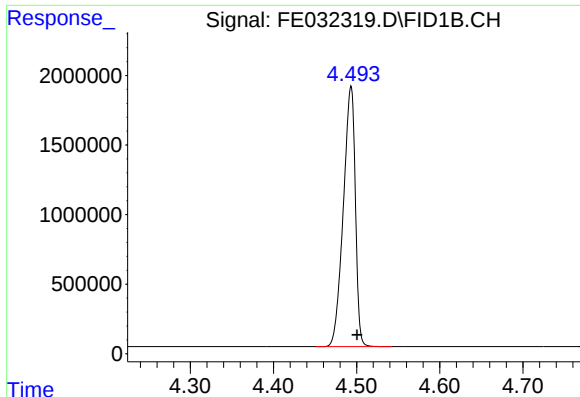


#2 N-DECANE

R.T.: 4.493 min
Delta R.T.: -0.007 min
Response: 18779346
Conc: 54.00 ug/ml

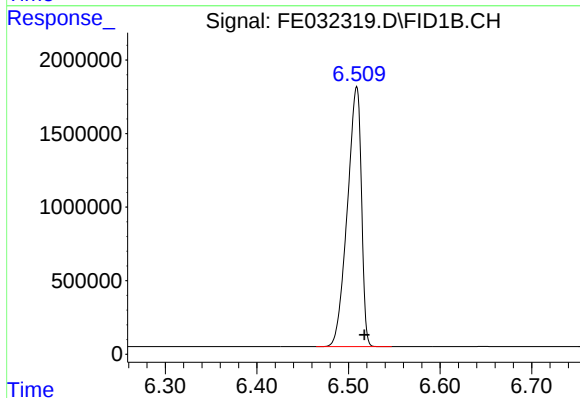


#3 N-DODECANE

R.T.: 6.509 min
Delta R.T.: -0.008 min
Response: 18863730
Conc: 54.05 ug/ml

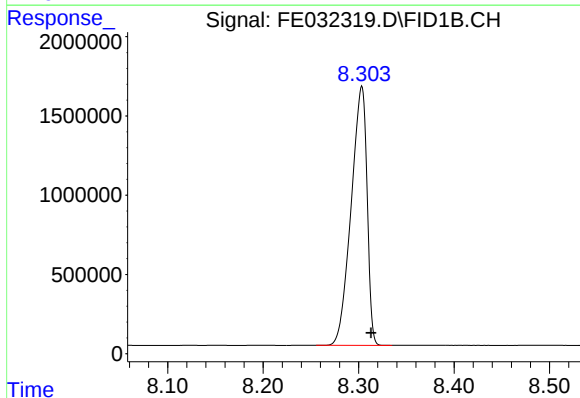


#4 N-TETRADECANE

R.T.: 8.303 min
Delta R.T.: -0.010 min
Response: 18850002
Conc: 54.24 ug/ml

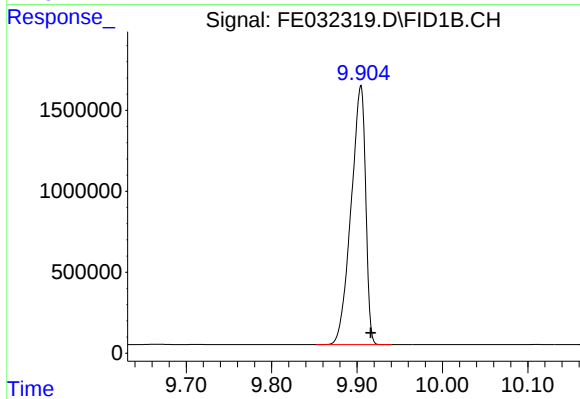


#5 N-HEXADECANE

R.T.: 9.905 min
Delta R.T.: -0.011 min
Response: 18931800
Conc: 54.30 ug/ml

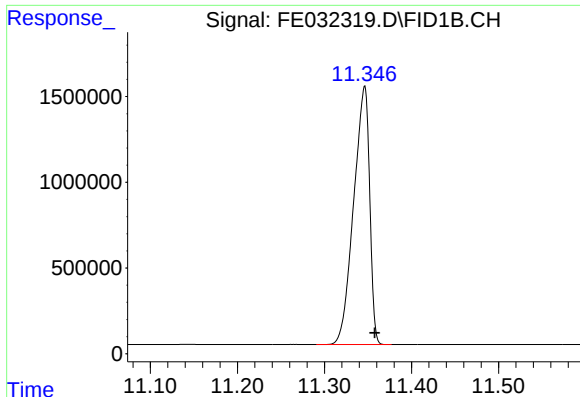


#6 N-OCTADECANE

R.T.: 11.346 min
Delta R.T.: -0.011 min
Response: 19194370
Conc: 54.28 ug/ml

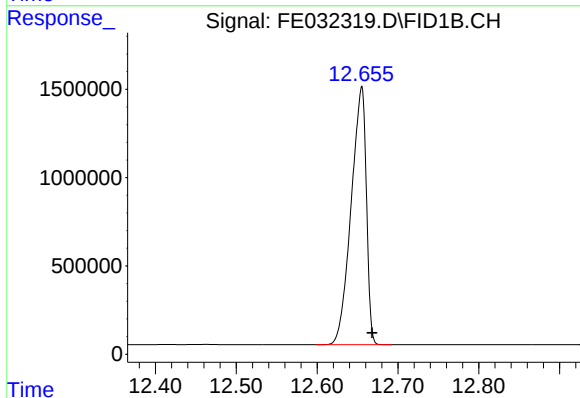


#7 N-EICOSANE

R.T.: 12.655 min
Delta R.T.: -0.013 min
Response: 19035339
Conc: 54.12 ug/ml

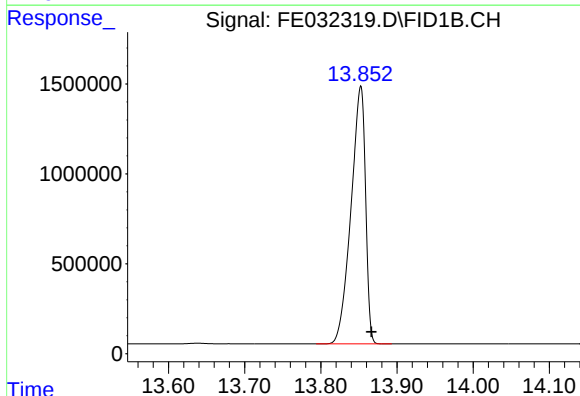


#8 N-DOCOSANE

R.T.: 13.853 min
Delta R.T.: -0.014 min
Response: 18954465
Conc: 53.94 ug/ml

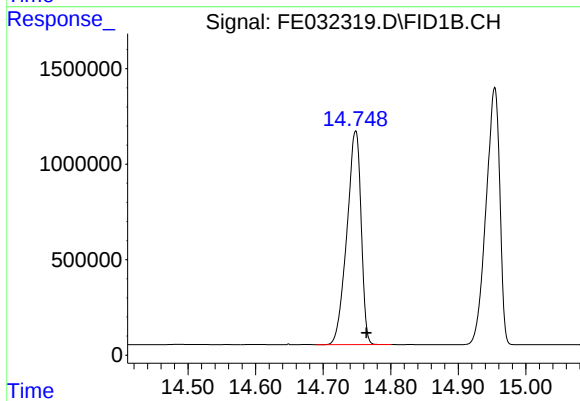


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.748 min
Delta R.T.: -0.016 min
Response: 16372975
Conc: 53.82 ug/ml

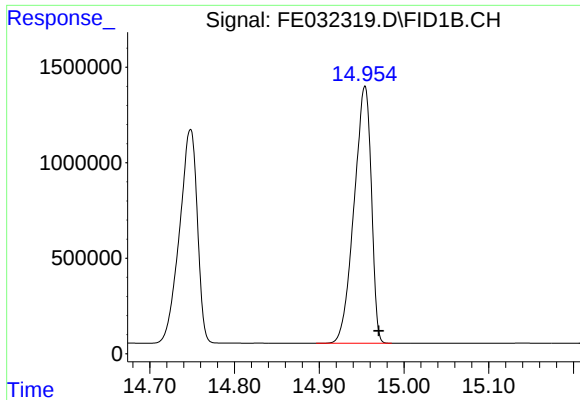


#10 N-TETRACOSANE

R.T.: 14.954 min
Delta R.T.: -0.016 min
Response: 19007965
Conc: 53.70 ug/ml

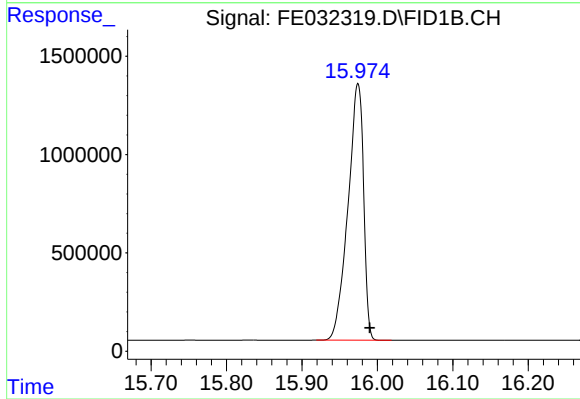

#11 N-HEXACOSANE

R.T.: 15.974 min
Delta R.T.: -0.015 min
Response: 18741969
Conc: 53.41 ug/ml

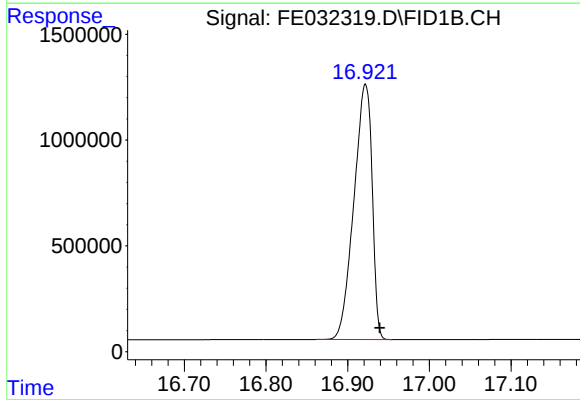

#12 N-OCTACOSANE

R.T.: 16.922 min
Delta R.T.: -0.017 min
Response: 18691757
Conc: 53.15 ug/ml