

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE070920\  
Data File : FE032323.D  
Signal(s) : FID1B.CH  
Acq On : 09 Jul 2020 9:57  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Integration File: Sample.e  
Quant Time: Jul 10 01:40:37 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE070720.M  
Quant Title :  
QLast Update : Wed Jul 08 12:04:06 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |              | R.T.   | Response | Conc Units   |
|-----------------------------|--------------|--------|----------|--------------|
| -----                       |              |        |          |              |
| System Monitoring Compounds |              |        |          |              |
| Target Compounds            |              |        |          |              |
| 3)                          | N-DODECANE   | 6.505  | 15693184 | 44.969 ug/ml |
| 12)                         | N-OCTACOSANE | 16.917 | 16095589 | 45.765 ug/ml |
| -----                       |              |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE070920\  
Data File : FE032323.D  
Signal(s) : FID1B.CH  
Acq On : 09 Jul 2020 9:57  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Integration File: Sample.e  
Quant Time: Jul 10 01:40:37 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE070720.M  
Quant Title :  
QLast Update : Wed Jul 08 12:04:06 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

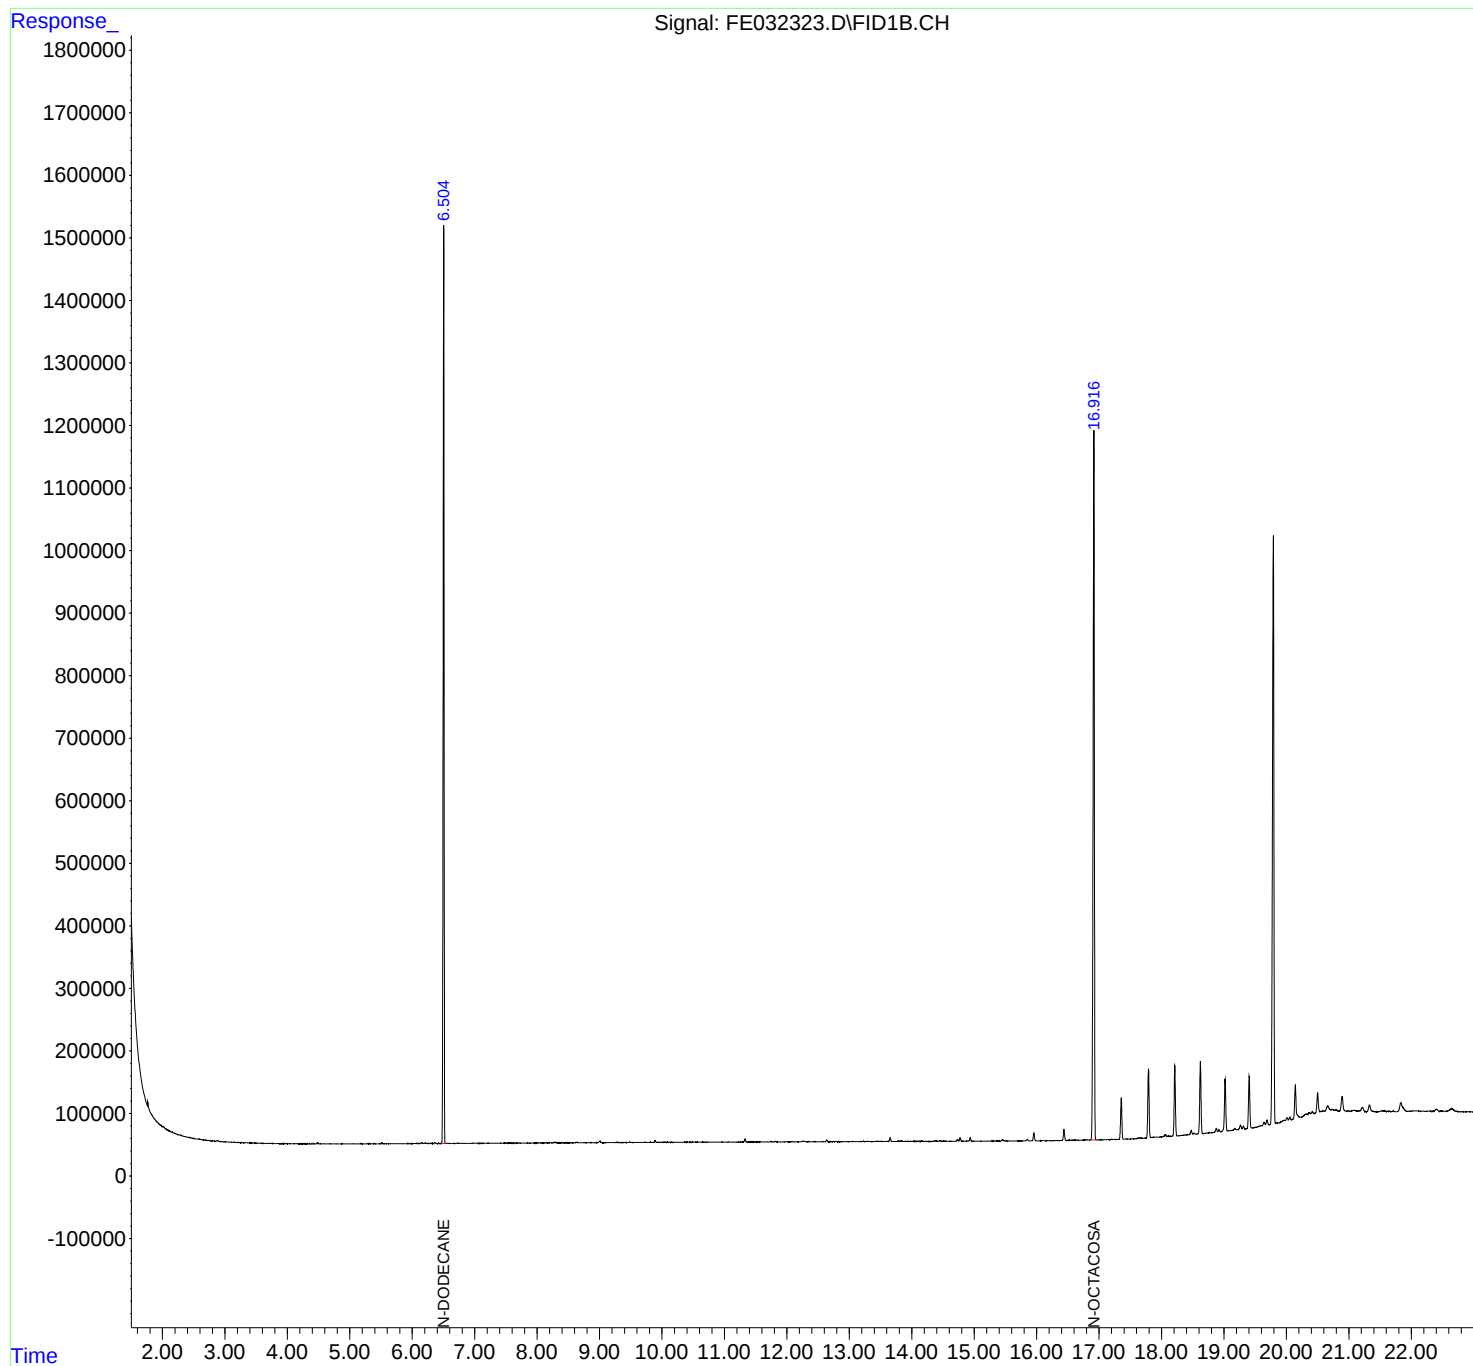

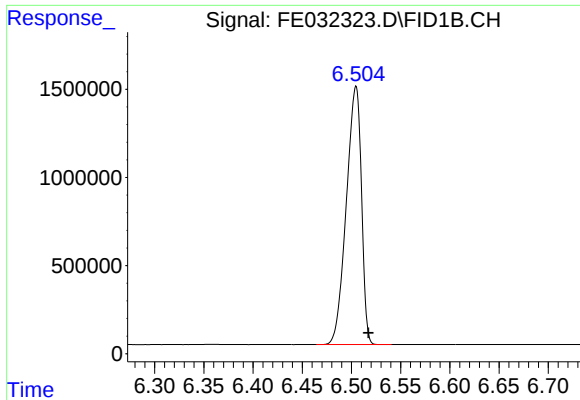


#3 N-DODECANE

R.T.: 6.505 min  
Delta R.T.: -0.013 min  
Response: 15693184  
Conc: 44.97 ug/ml

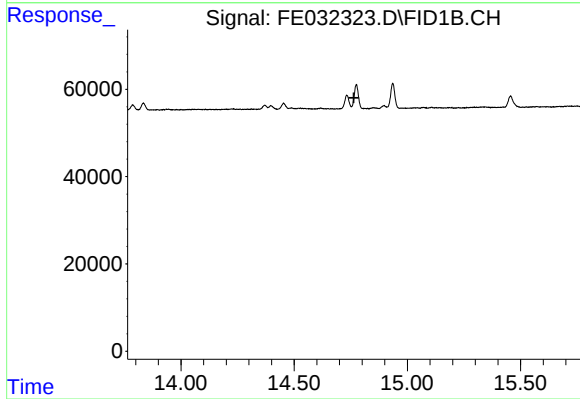

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.764 min  
Response: 0  
Conc: N.D.

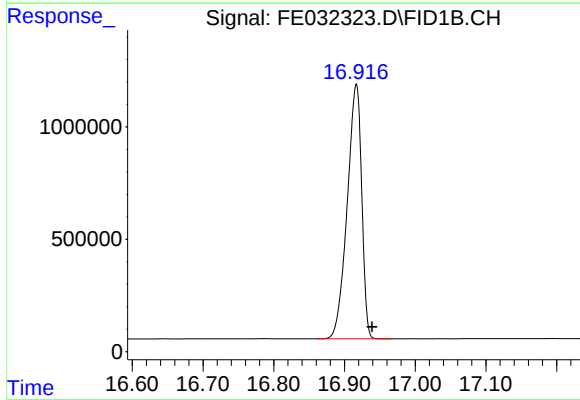

#12 N-OCTACOSANE

R.T.: 16.917 min  
Delta R.T.: -0.022 min  
Response: 16095589  
Conc: 45.77 ug/ml