

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070920\
 Data File : FE032333.D
 Signal(s) : FID1B.CH
 Acq On : 09 Jul 2020 15:45
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
 Quant Time: Jul 10 01:42:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE070720.M
 Quant Title :
 QLast Update : Wed Jul 08 12:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.745	14959569	49.174 ug/ml
Target Compounds			
2) N-DECANE	4.492	17217111	49.506 ug/ml
3) N-DODECANE	6.507	17233215	49.382 ug/ml
4) N-TETRADECANE	8.301	17145549	49.338 ug/ml
5) N-HEXADECANE	9.902	17207922	49.357 ug/ml
6) N-OCTADECANE	11.342	17475045	49.417 ug/ml
7) N-EICOSANE	12.652	17363477	49.371 ug/ml
8) N-DOCOSANE	13.848	17297858	49.227 ug/ml
10) N-TETRACOSANE	14.952	17349502	49.013 ug/ml
11) N-HEXACOSANE	15.970	17104300	48.742 ug/ml
12) N-OCTACOSANE	16.918	17035411	48.438 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070920\
Data File : FE032333.D
Signal(s) : FID1B.CH
Acq On : 09 Jul 2020 15:45
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: Sample.e
Quant Time: Jul 10 01:42:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE070720.M
Quant Title :
QLast Update : Wed Jul 08 12:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

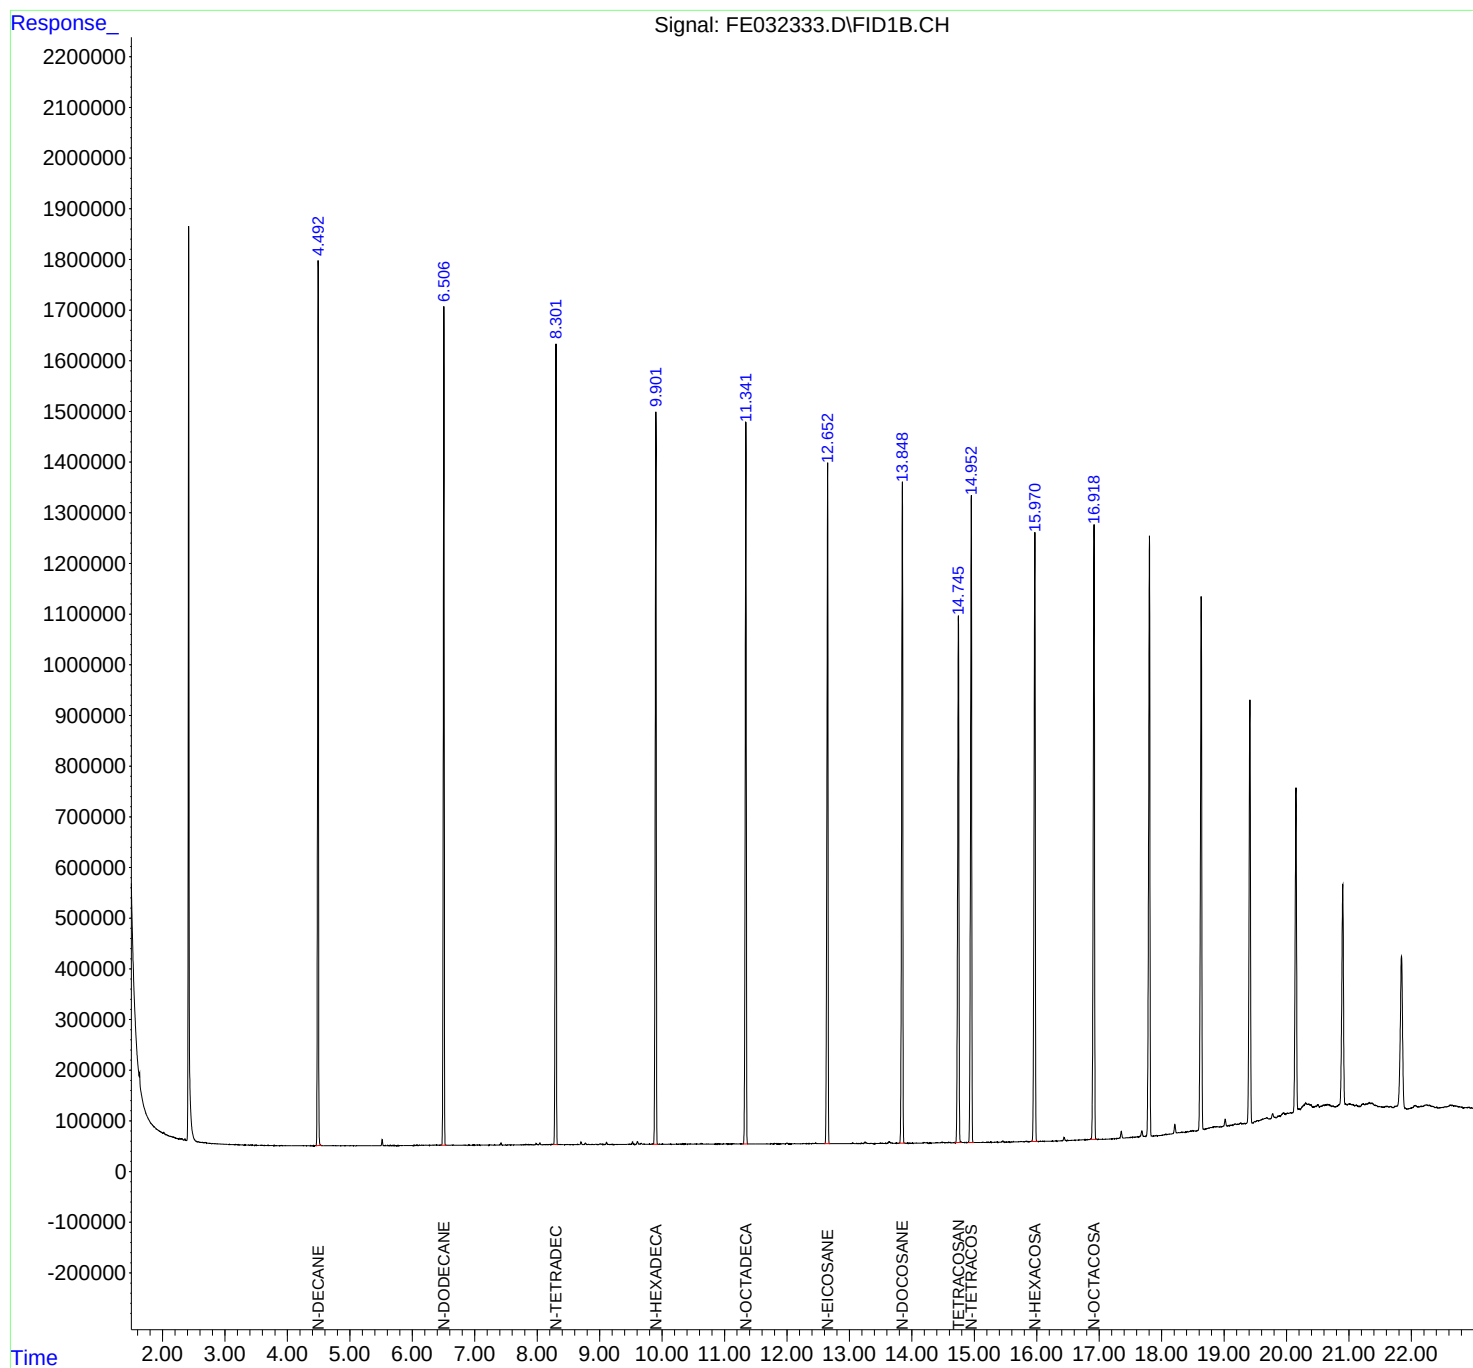

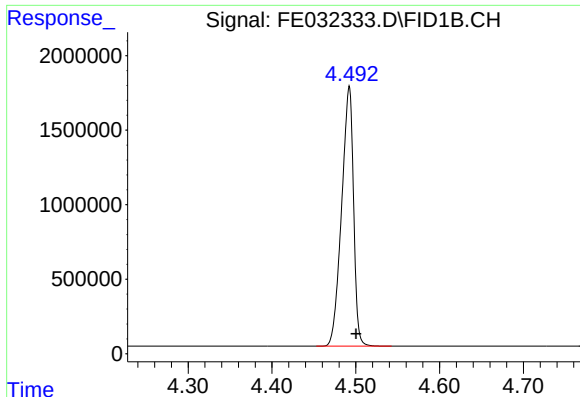


#2 N-DECANE

R.T.: 4.492 min
Delta R.T.: -0.008 min
Response: 17217111
Conc: 49.51 ug/ml

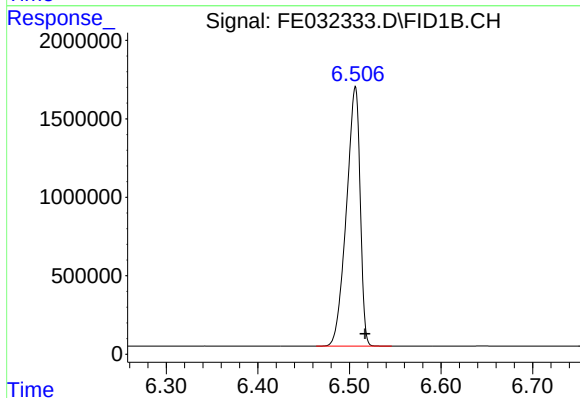


#3 N-DODECANE

R.T.: 6.507 min
Delta R.T.: -0.011 min
Response: 17233215
Conc: 49.38 ug/ml

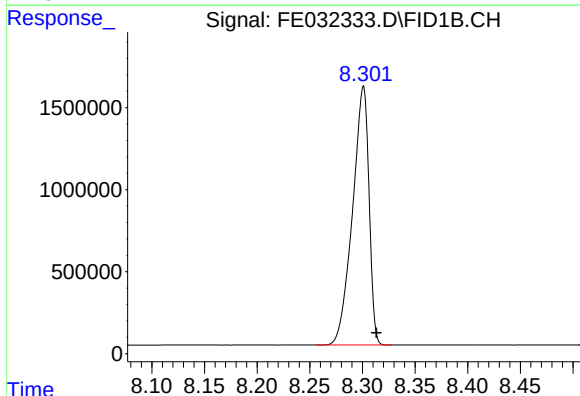


#4 N-TETRADECANE

R.T.: 8.301 min
Delta R.T.: -0.012 min
Response: 17145549
Conc: 49.34 ug/ml

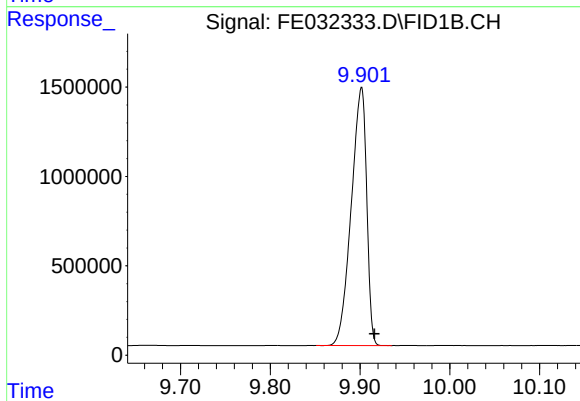


#5 N-HEXADECANE

R.T.: 9.902 min
Delta R.T.: -0.014 min
Response: 17207922
Conc: 49.36 ug/ml

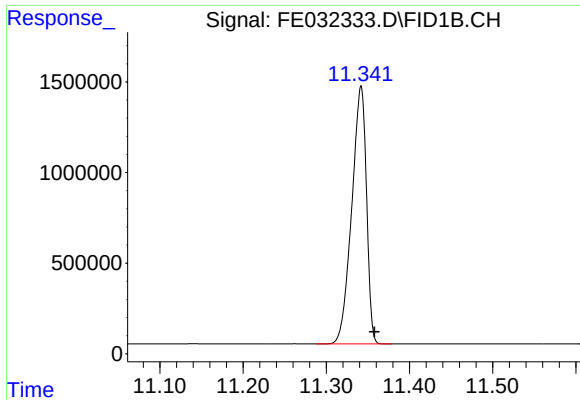


#6 N-OCTADECANE

R.T.: 11.342 min
Delta R.T.: -0.016 min
Response: 17475045
Conc: 49.42 ug/ml

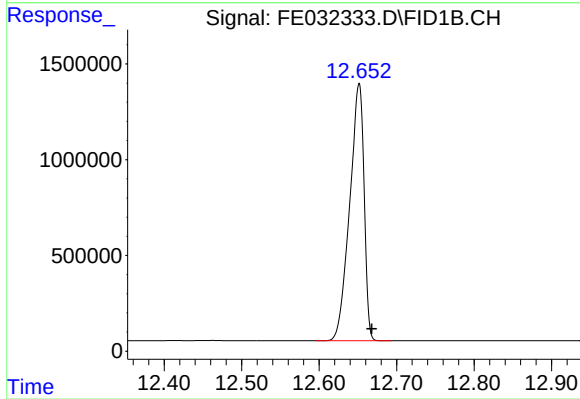


#7 N-EICOSANE

R.T.: 12.652 min
Delta R.T.: -0.016 min
Response: 17363477
Conc: 49.37 ug/ml

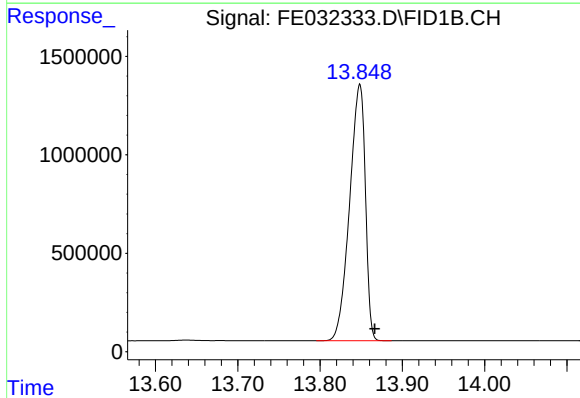


#8 N-DOCOSANE

R.T.: 13.848 min
Delta R.T.: -0.018 min
Response: 17297858
Conc: 49.23 ug/ml

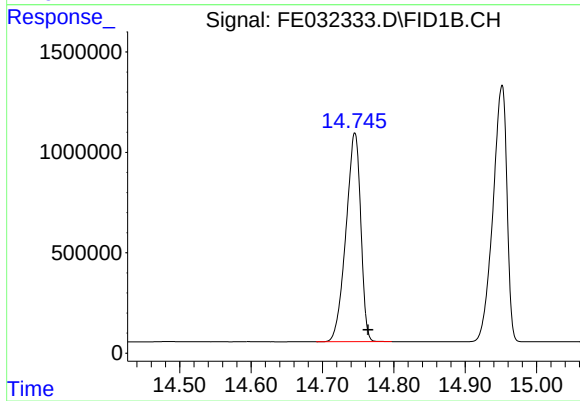


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.745 min
Delta R.T.: -0.019 min
Response: 14959569
Conc: 49.17 ug/ml

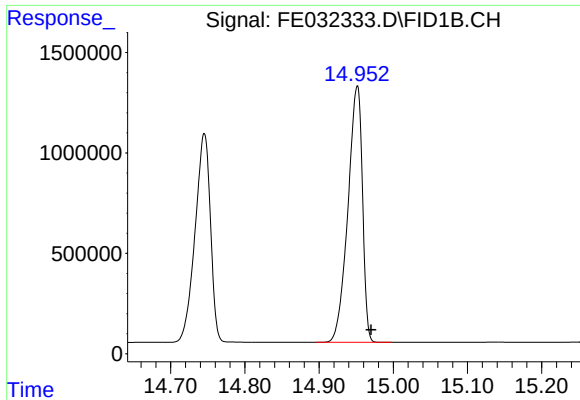


#10 N-TETRACOSANE

R.T.: 14.952 min
Delta R.T.: -0.018 min
Response: 17349502
Conc: 49.01 ug/ml

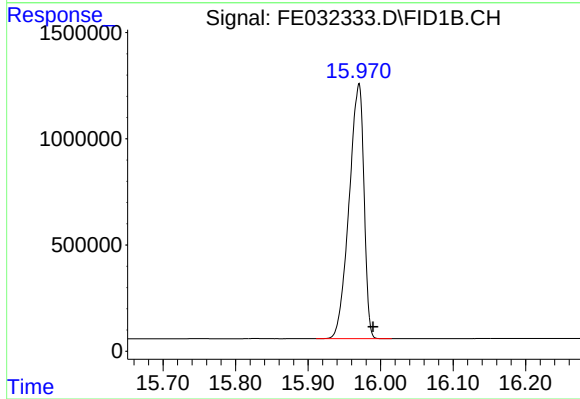

#11 N-HEXACOSANE

R.T.: 15.970 min
Delta R.T.: -0.020 min
Response: 17104300
Conc: 48.74 ug/ml

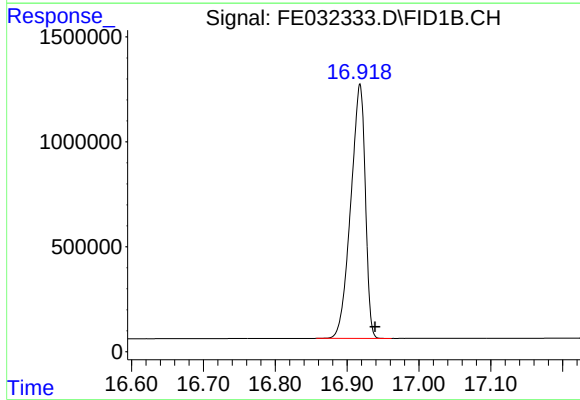

#12 N-OCTACOSANE

R.T.: 16.918 min
Delta R.T.: -0.021 min
Response: 17035411
Conc: 48.44 ug/ml