

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071122\
Data File : FE036443.D
Signal(s) : FID1B.ch
Acq On : 11 Jul 2022 10:03
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 12 01:04:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE062022.M
Quant Title :
QLast Update : Tue Jun 21 02:15:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.947	2477069	17.653 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.837	121804	0.863 ug/ml
15) N-TETRATRIACONTANE	19.599	16373	0.127 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071122\
Data File : FE036443.D
Signal(s) : FID1B.ch
Acq On : 11 Jul 2022 10:03
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 12 01:04:44 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE062022.M
Quant Title :
QLast Update : Tue Jun 21 02:15:59 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

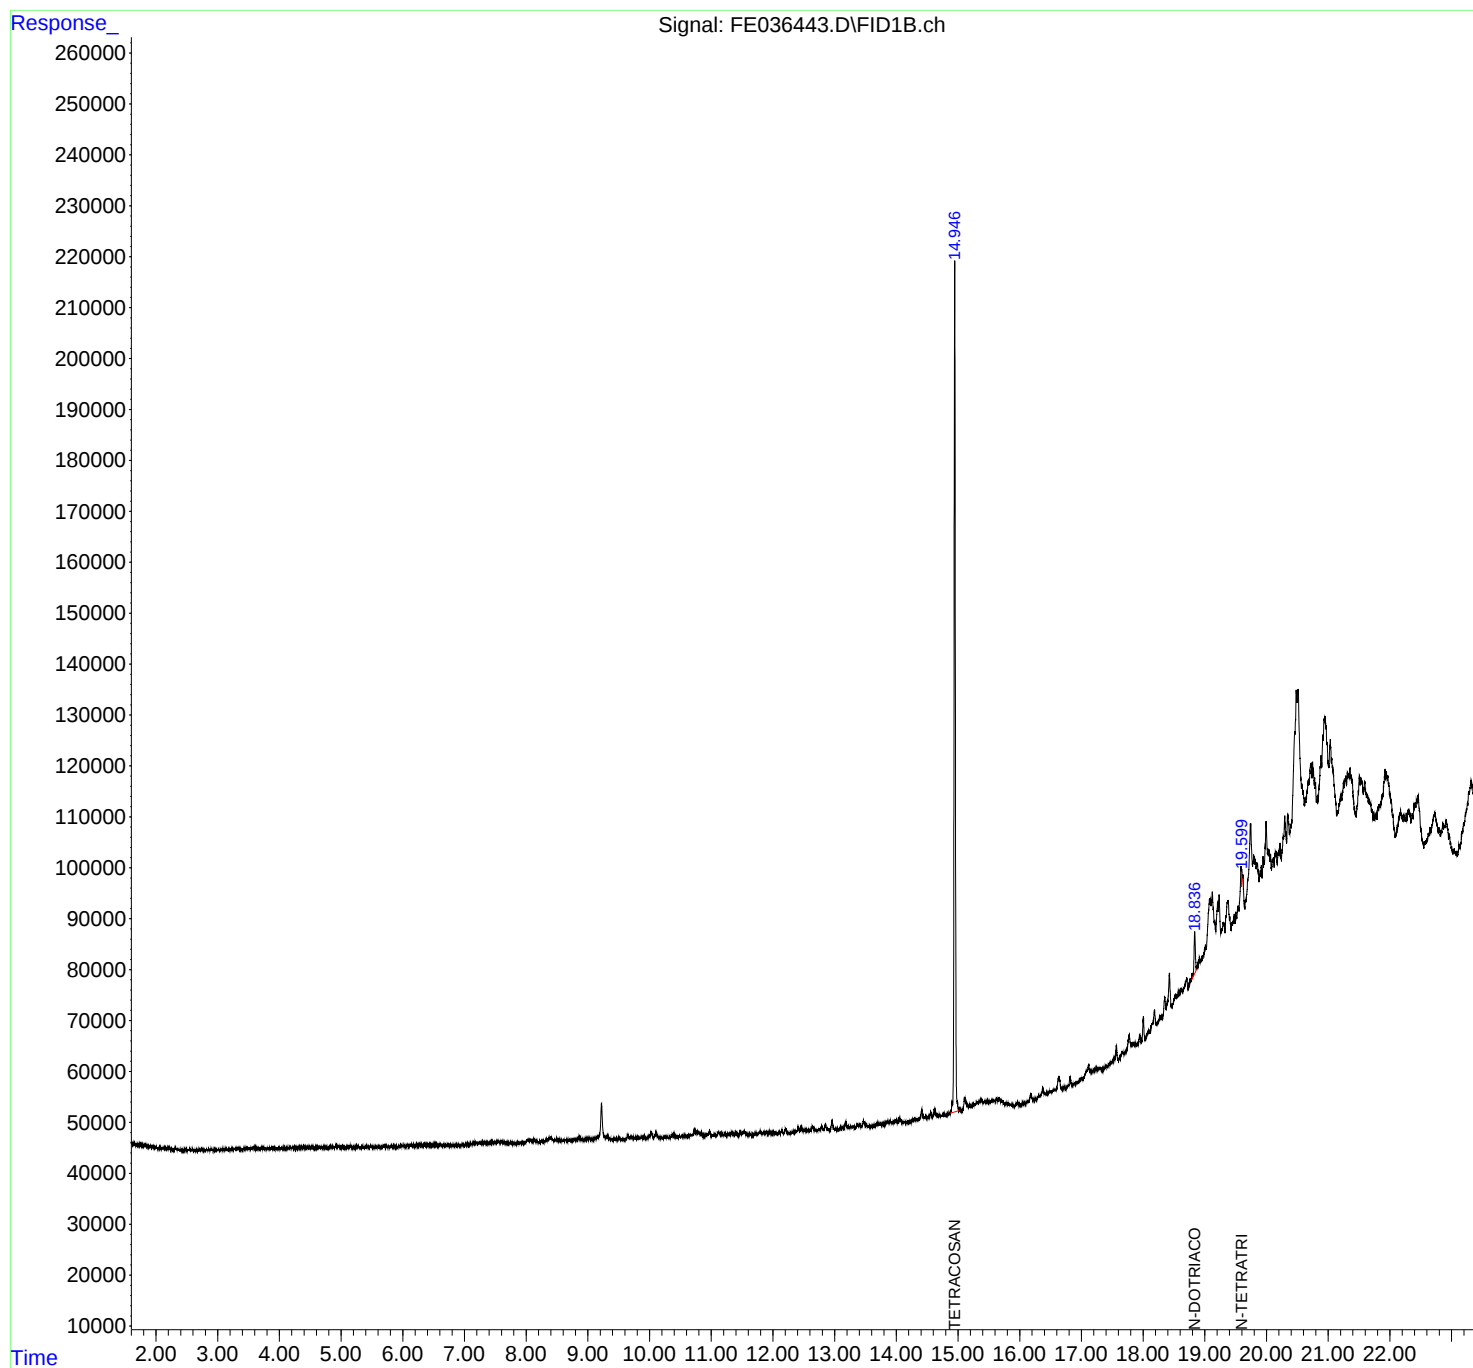

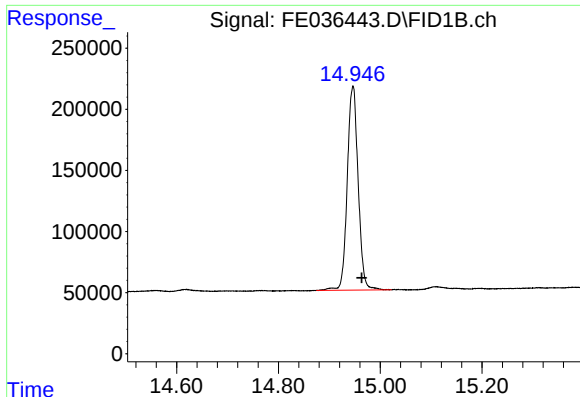


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.947 min
Delta R.T.: -0.017 min
Response: 2477069
Conc: 17.65 ug/ml

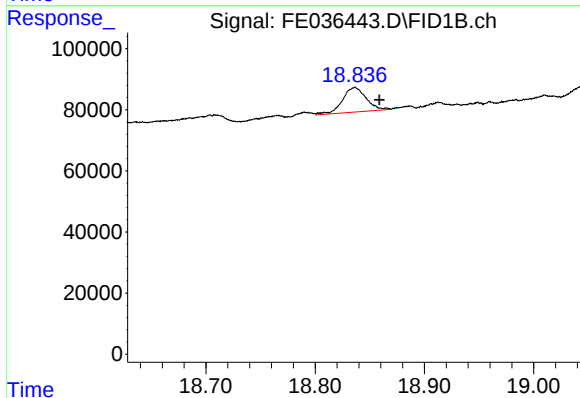

#14 N-DOTRIACONTANE

R.T.: 18.837 min
Delta R.T.: -0.022 min
Response: 121804
Conc: 0.86 ug/ml

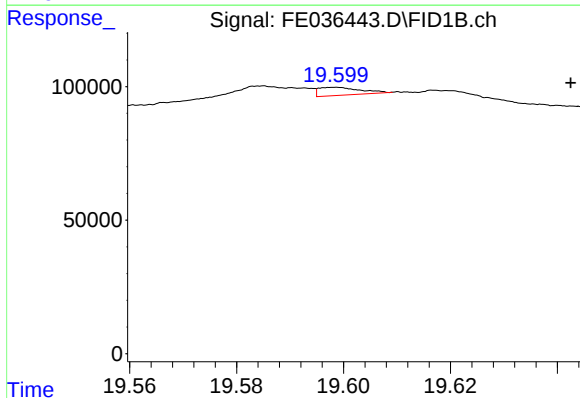

#15 N-TETRATRIACONTANE

R.T.: 19.599 min
Delta R.T.: -0.044 min
Response: 16373
Conc: 0.13 ug/ml