

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071219\
 Data File : FE030134.D
 Signal(s) : FID1B.CH
 Acq On : 12 Jul 2019 12:51
 Operator : AJ\SJ
 Sample : K3768-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 13 00:10:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062019.M
 Quant Title :
 QLast Update : Thu Jun 20 13:12:27 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.592	2665974	13.440 ug/ml
Target Compounds				
10)	N-TETRACOSANE	14.803	109856	0.562 ug/ml
11)	N-OCTACOSANE	16.767	519203	2.696 ug/ml
12)	N-DOTRIACONTANE	18.487	476721	2.571 ug/ml
14)	N-HEXATRIACONTANE	20.013	74961	0.457 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071219\
Data File : FE030134.D
Signal(s) : FID1B.CH
Acq On : 12 Jul 2019 12:51
Operator : AJ\SJ
Sample : K3768-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 13 00:10:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062019.M
Quant Title :
QLast Update : Thu Jun 20 13:12:27 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

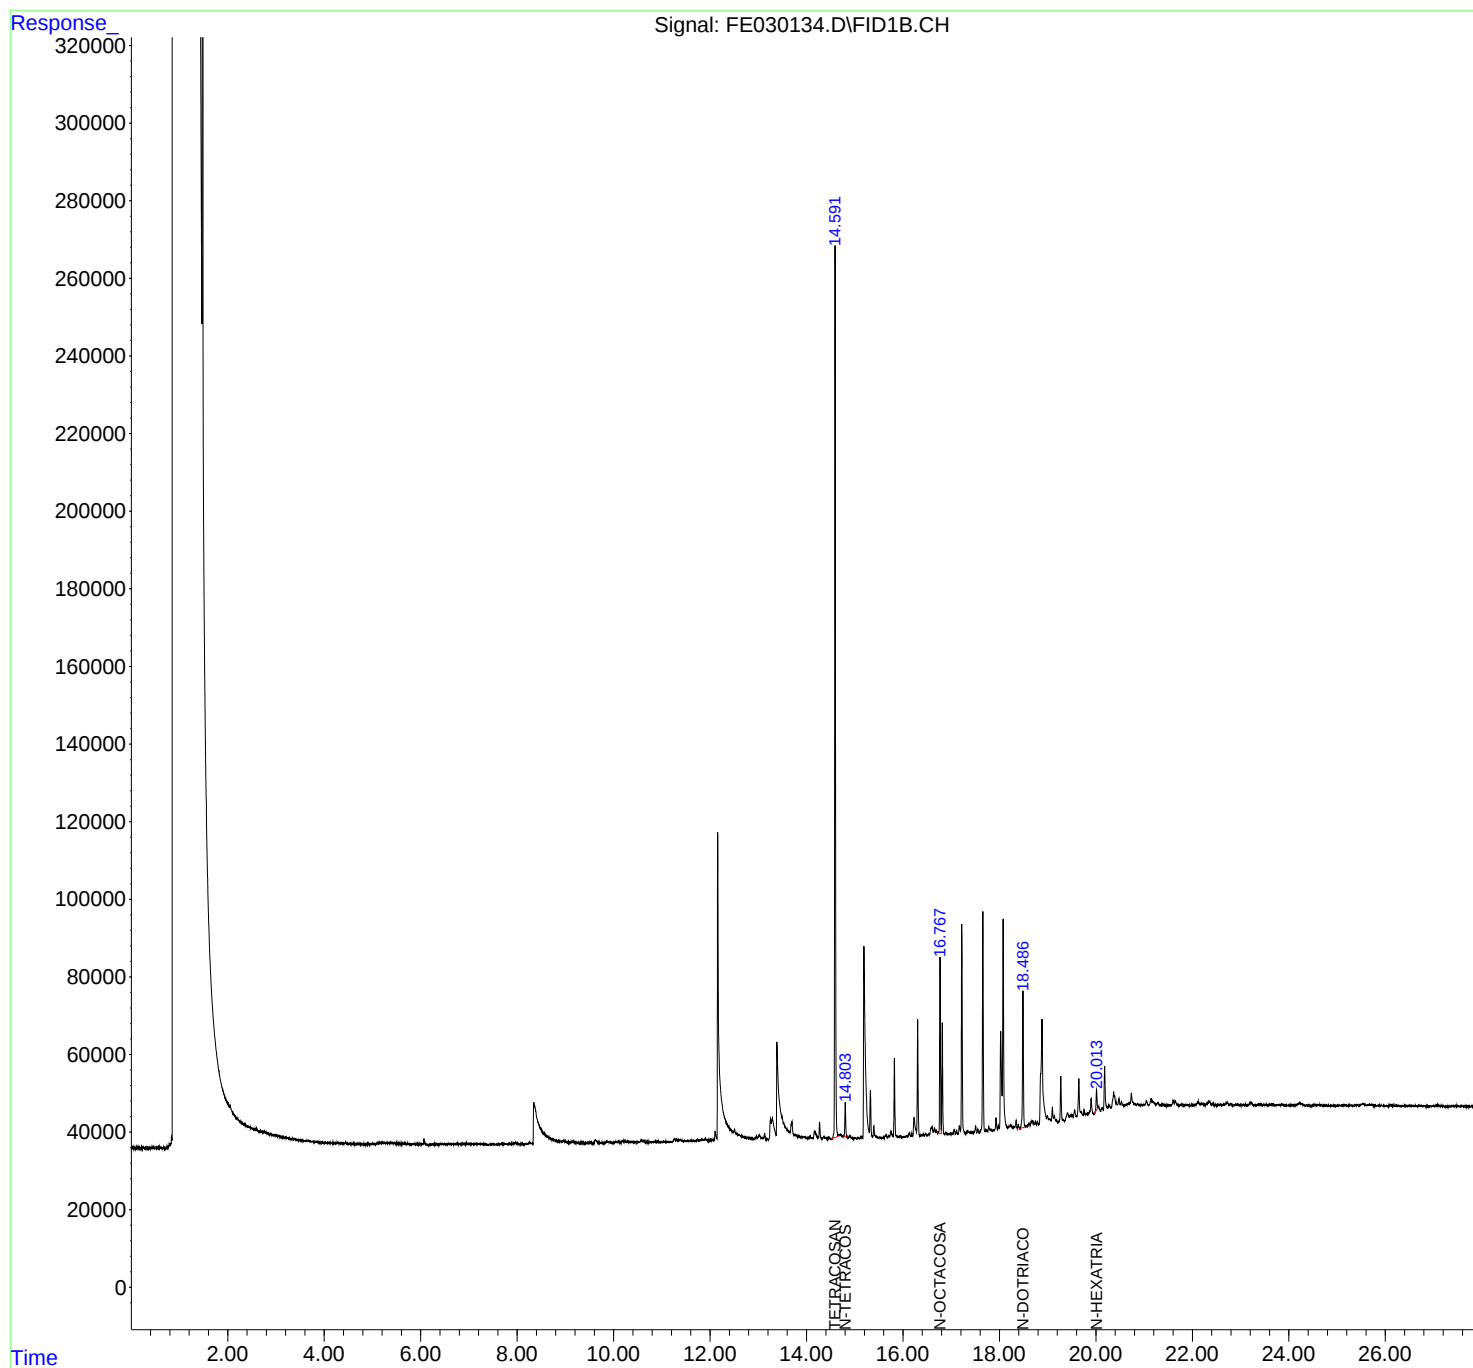

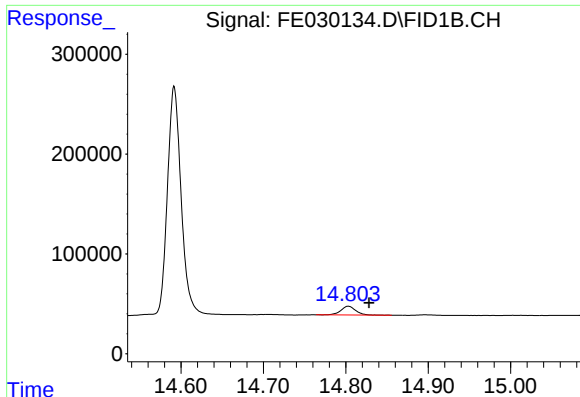


#10 N-TETRACOSANE

R.T.: 14.803 min
Delta R.T.: -0.025 min
Response: 109856
Conc: 0.56 ug/ml

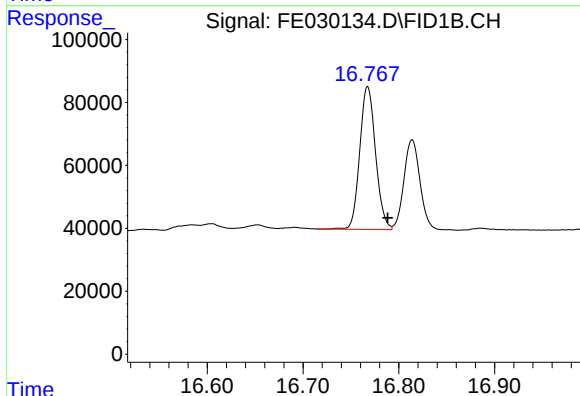


#11 N-OCTACOSANE

R.T.: 16.767 min
Delta R.T.: -0.021 min
Response: 519203
Conc: 2.70 ug/ml

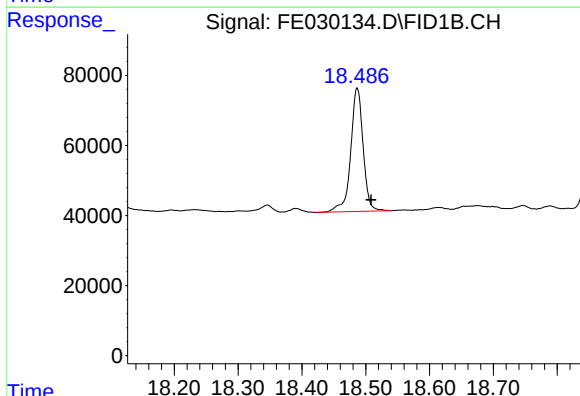


#12 N-DOTRIACONTANE

R.T.: 18.487 min
Delta R.T.: -0.022 min
Response: 476721
Conc: 2.57 ug/ml

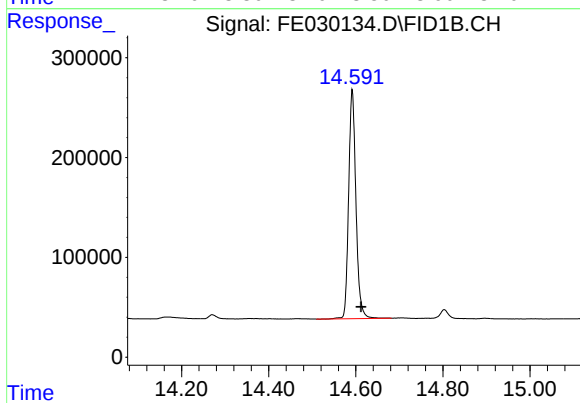

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.592 min
Delta R.T.: -0.020 min
Response: 2665974
Conc: 13.44 ug/ml

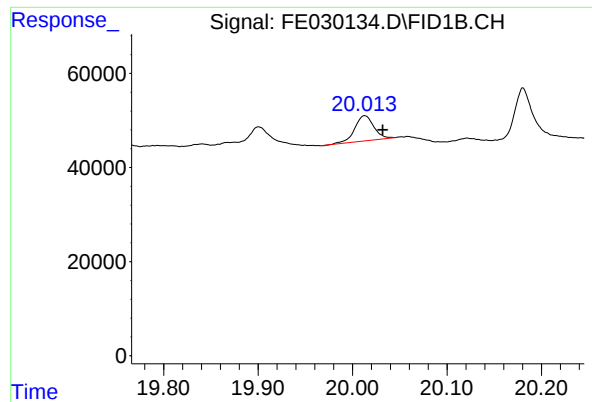

#14 N-HEXATRIACONTANE

R.T.: 20.013 min
Delta R.T.: -0.019 min
Response: 74961
Conc: 0.46 ug/ml