

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE071222\  
Data File : FE036453.D  
Signal(s) : FID1B.ch  
Acq On : 12 Jul 2022 08:50  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Jul 13 01:20:05 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE062022.M  
Quant Title :  
QLast Update : Tue Jun 21 02:15:59 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.945	2458089	17.517 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.832	108455	0.769 ug/ml
-----			


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE071222\  
Data File : FE036453.D  
Signal(s) : FID1B.ch  
Acq On : 12 Jul 2022 08:50  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Jul 13 01:20:05 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE062022.M  
Quant Title :  
QLast Update : Tue Jun 21 02:15:59 2022  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

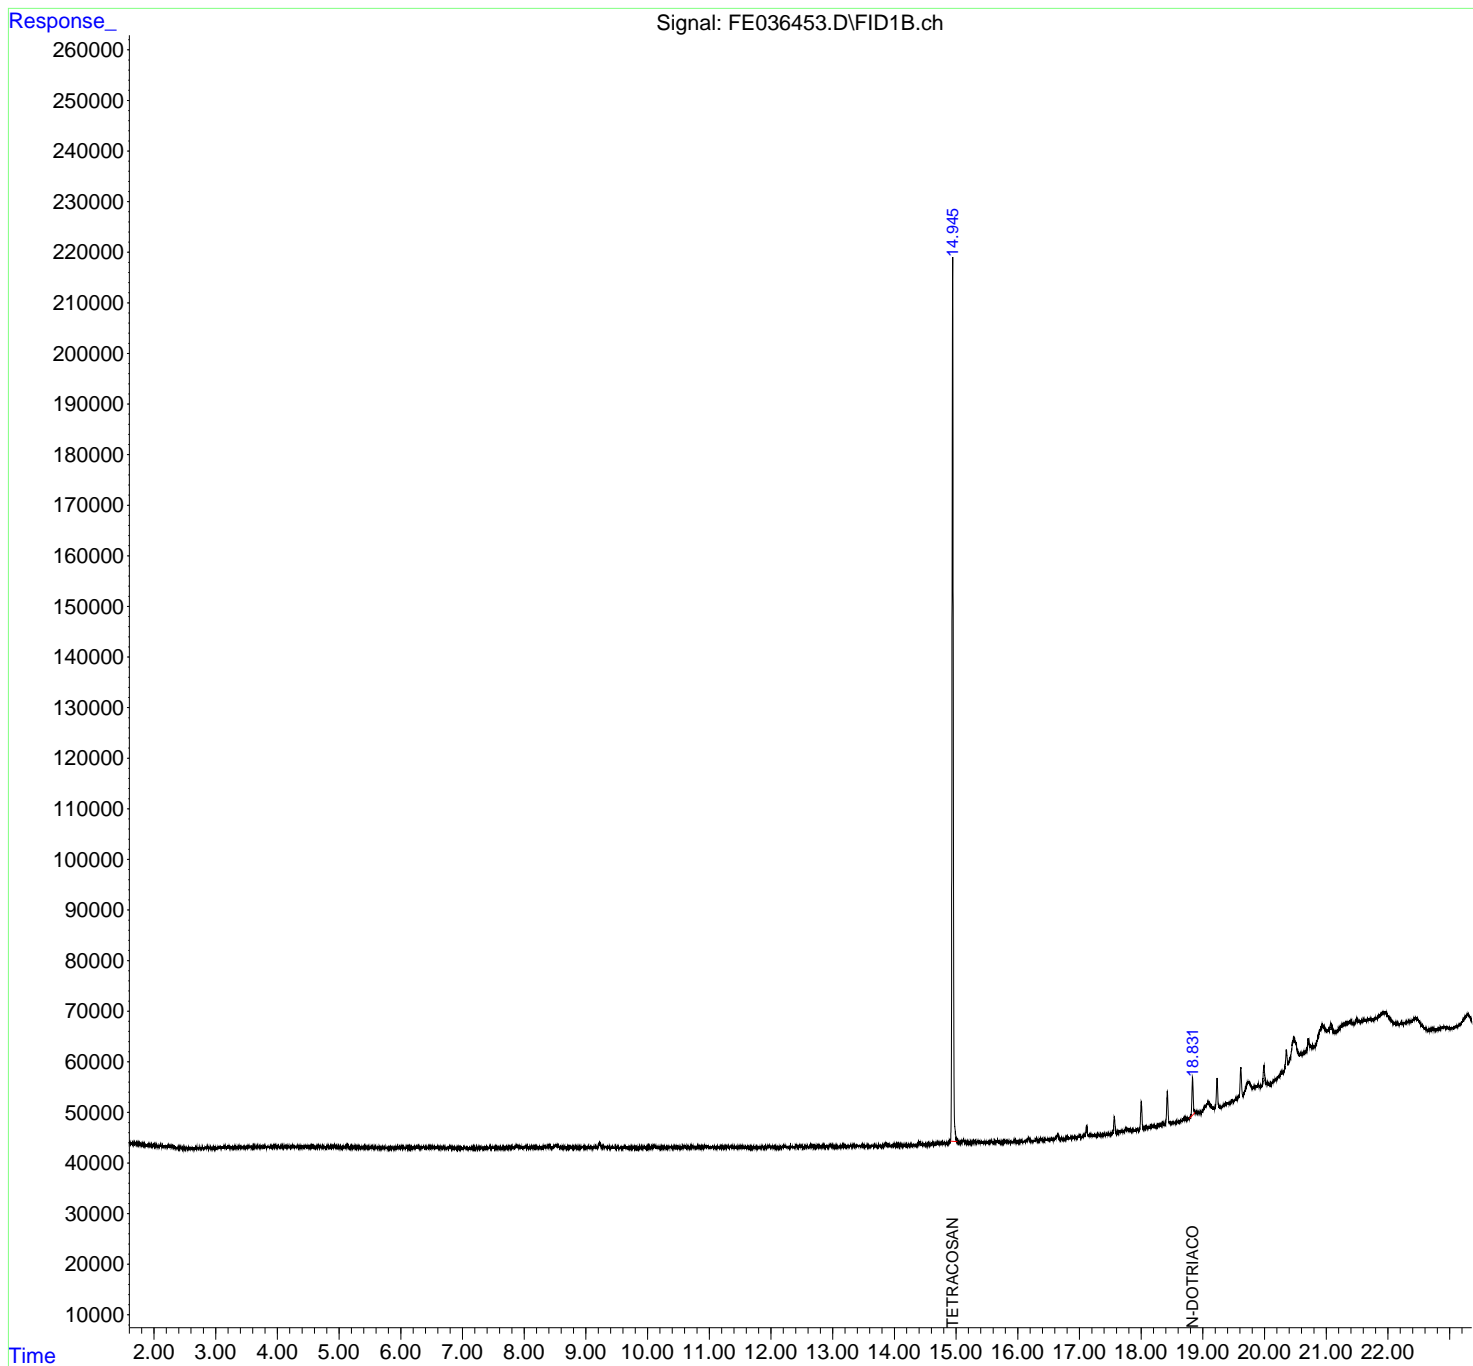

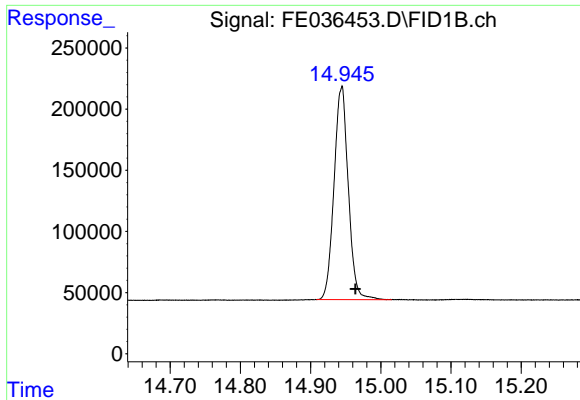

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.945 min  
Delta R.T.: -0.018 min  
Response: 2458089  
Conc: 17.52 ug/ml

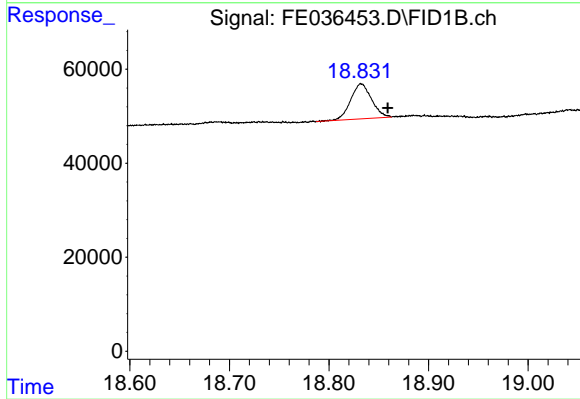

#14 N-DOTRIACONTANE

R.T.: 18.832 min  
Delta R.T.: -0.027 min  
Response: 108455  
Conc: 0.77 ug/ml