

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071222\
Data File : FE036464.D
Signal(s) : FID1B.ch
Acq On : 12 Jul 2022 14:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 13 01:22:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE062022.M
Quant Title :
QLast Update : Tue Jun 21 02:15:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.945	2378524	16.950 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.832	115229	0.817 ug/ml
15) N-TETRATRIACONTANE	19.615	98893	0.769 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071222\
Data File : FE036464.D
Signal(s) : FID1B.ch
Acq On : 12 Jul 2022 14:50
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 13 01:22:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE062022.M
Quant Title :
QLast Update : Tue Jun 21 02:15:59 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

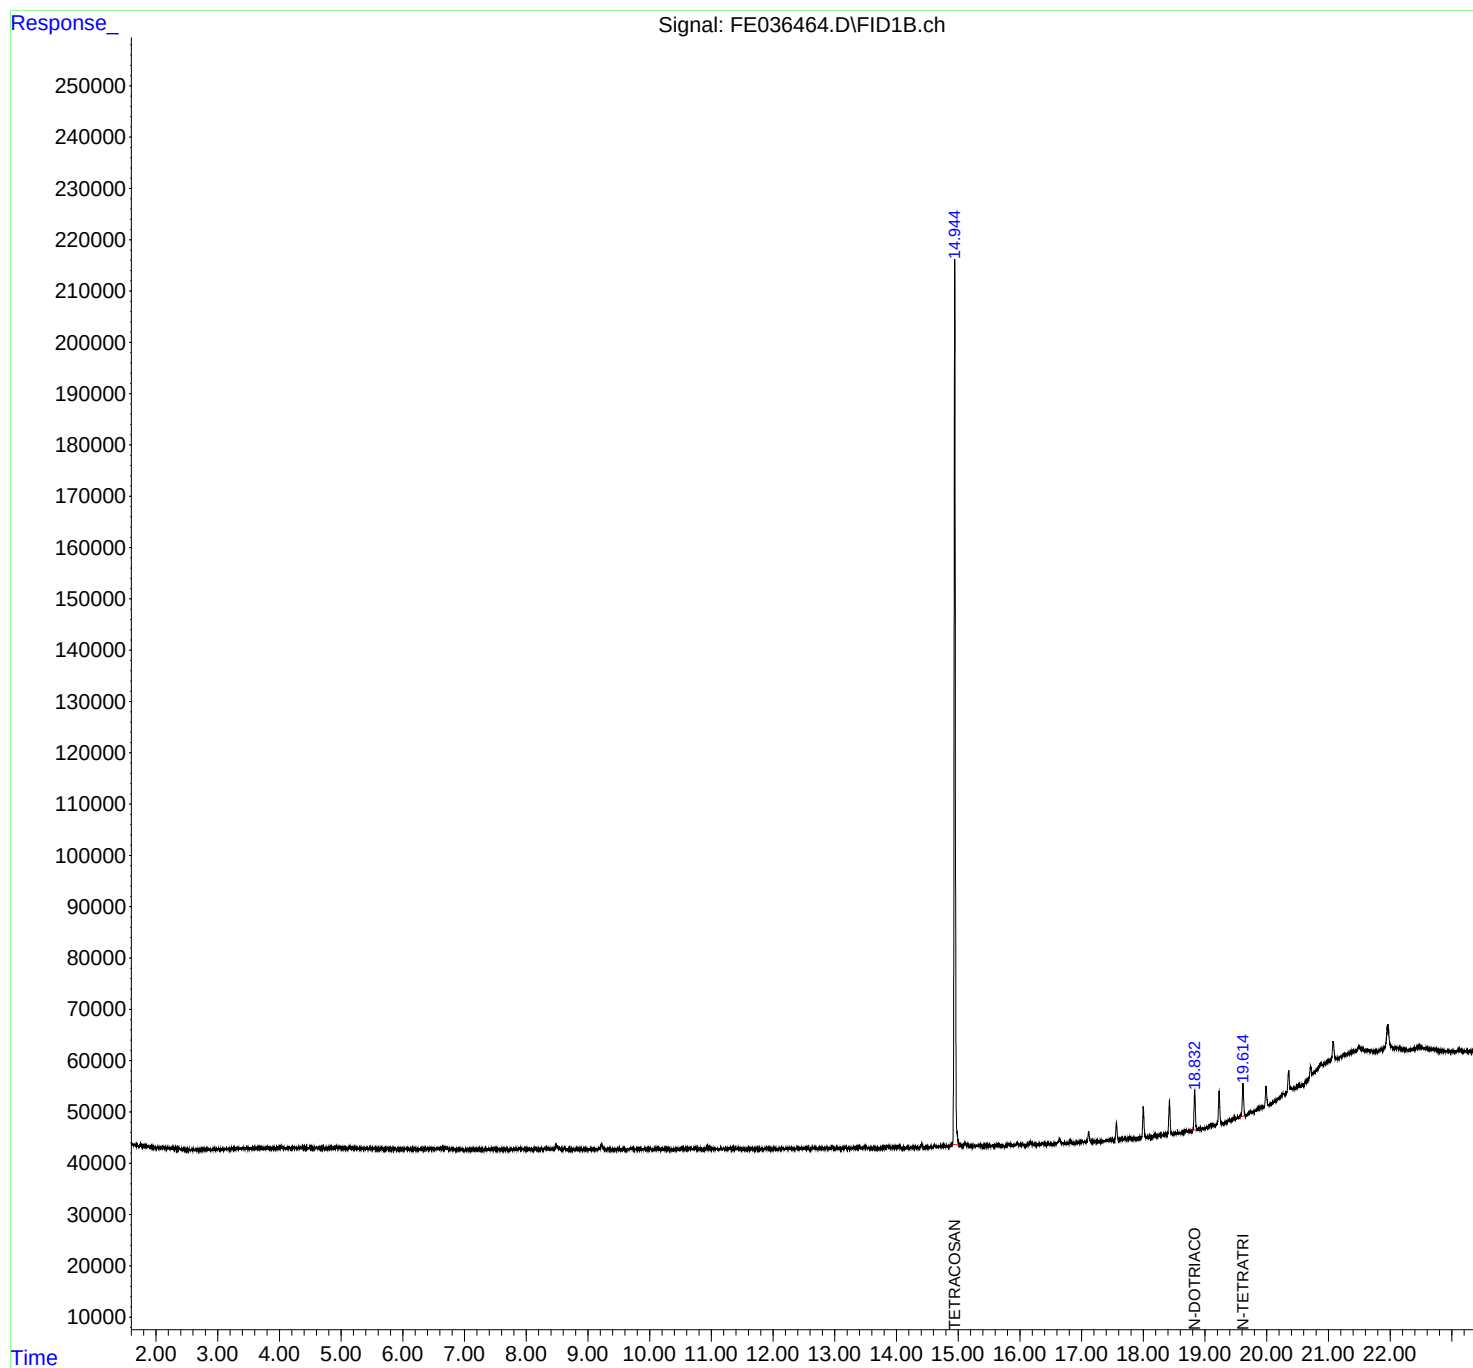

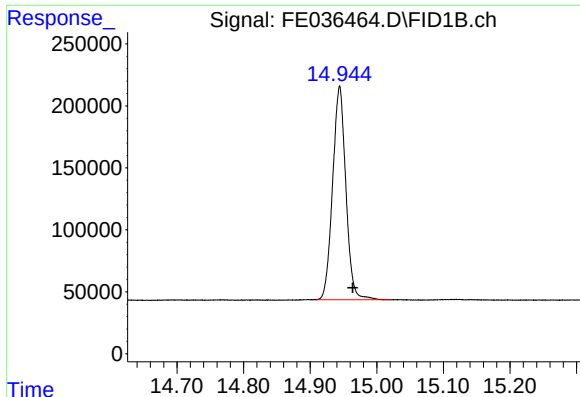


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.945 min
Delta R.T.: -0.019 min
Response: 2378524
Conc: 16.95 ug/ml

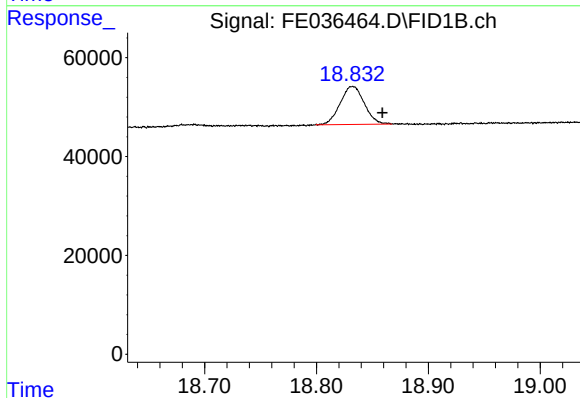

#14 N-DOTRIACONTANE

R.T.: 18.832 min
Delta R.T.: -0.026 min
Response: 115229
Conc: 0.82 ug/ml

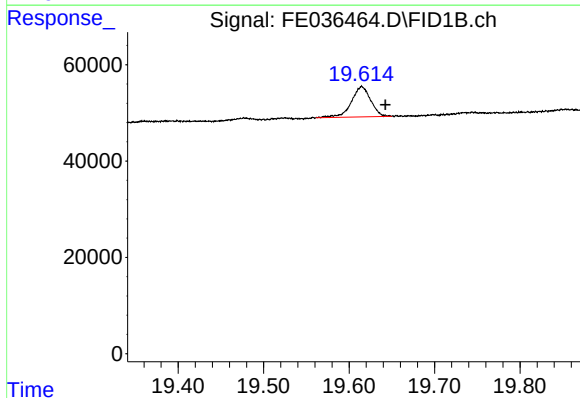

#15 N-TETRATRIACONTANE

R.T.: 19.615 min
Delta R.T.: -0.028 min
Response: 98893
Conc: 0.77 ug/ml