

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE071322\  
 Data File : FE036470.D  
 Signal(s) : FID1B.ch  
 Acq On : 13 Jul 2022 11:25  
 Operator : YP\AJ  
 Sample : PB145927BL  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Integration File: autoint1.e  
 Quant Time: Jul 14 01:22:04 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE062022.M  
 Quant Title :  
 QLast Update : Tue Jun 21 02:15:59 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.946	2015573	14.364 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.839	117038	0.830 ug/ml
-----			


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE071322\  
Data File : FE036470.D  
Signal(s) : FID1B.ch  
Acq On : 13 Jul 2022 11:25  
Operator : YP\AJ  
Sample : PB145927BL  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Jul 14 01:22:04 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE062022.M  
Quant Title :  
QLast Update : Tue Jun 21 02:15:59 2022  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

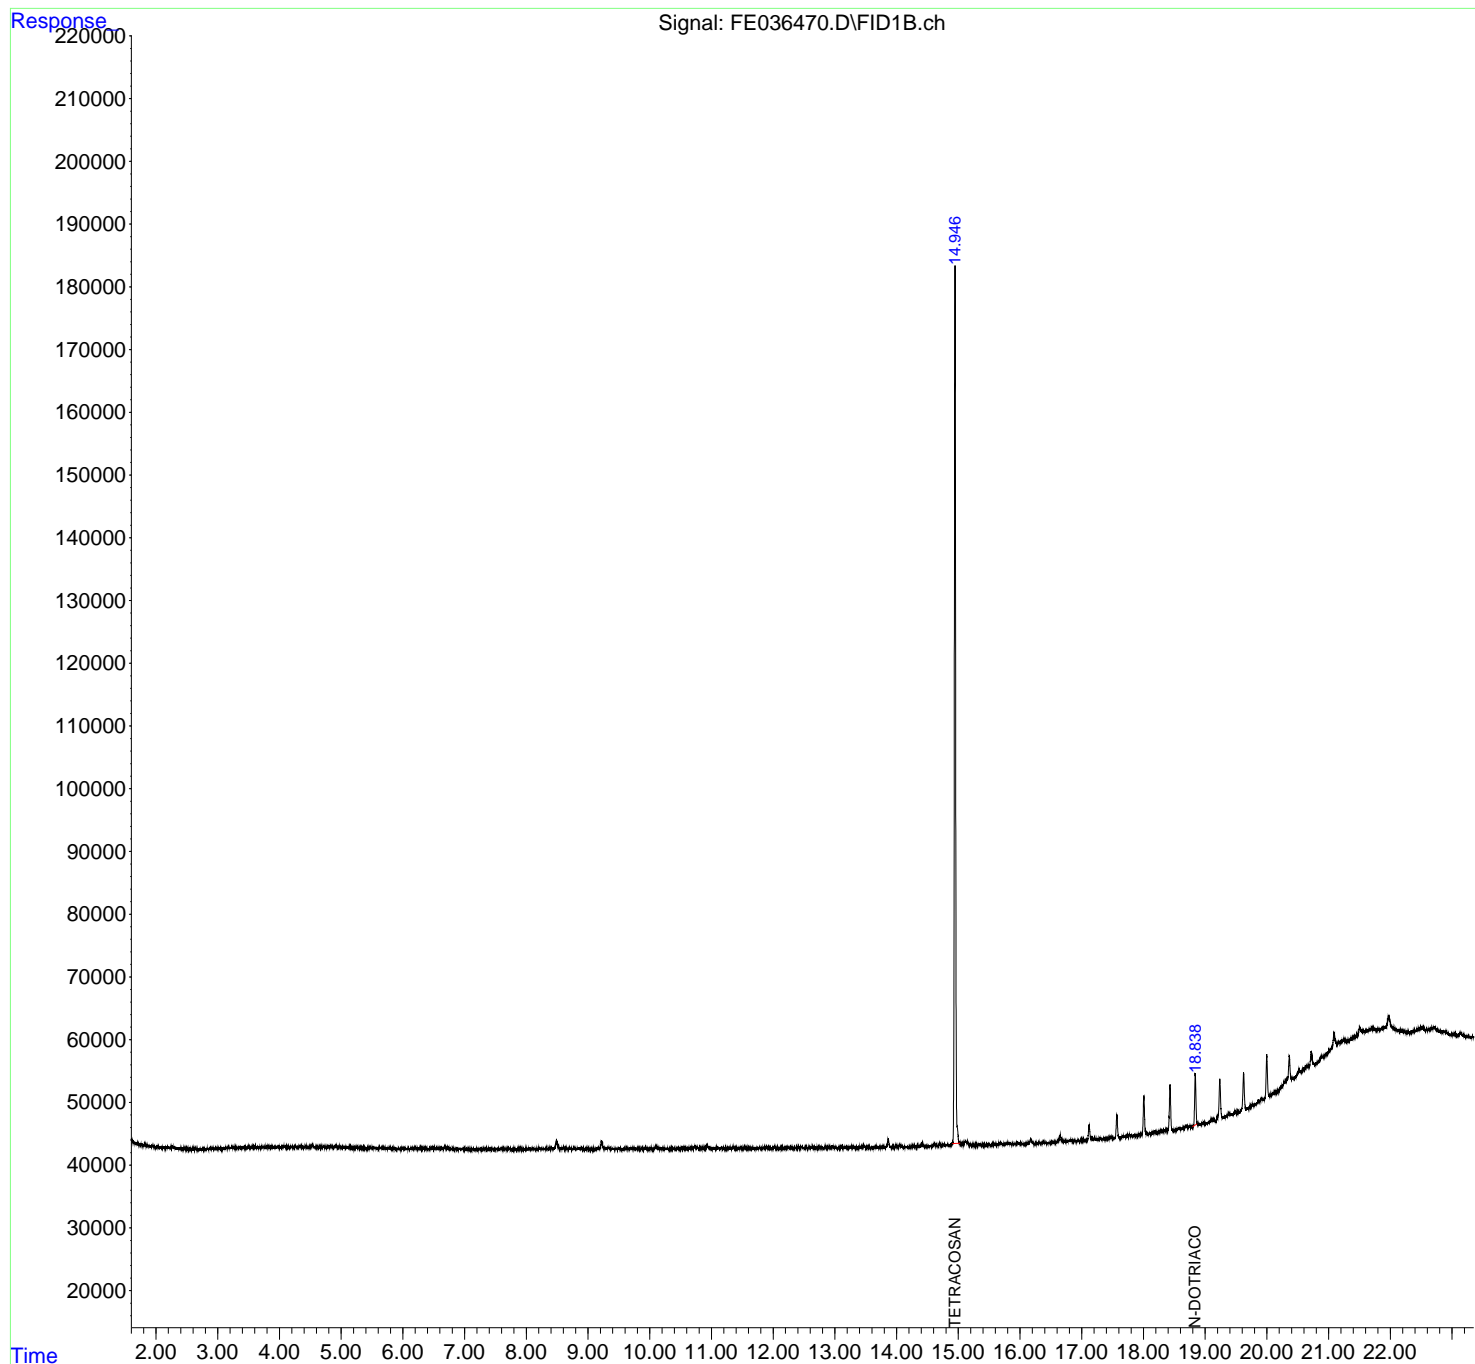

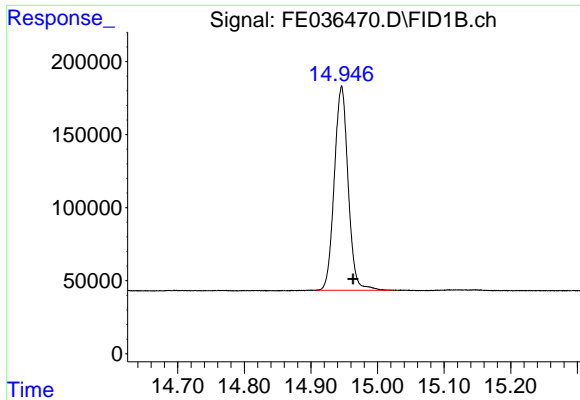

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.946 min  
Delta R.T.: -0.017 min  
Response: 2015573  
Conc: 14.36 ug/ml

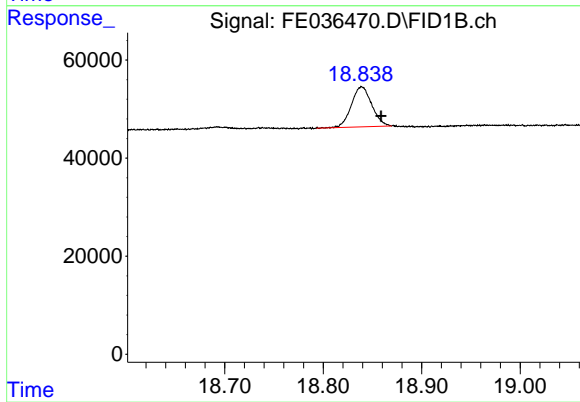

#14 N-DOTRIACONTANE

R.T.: 18.839 min  
Delta R.T.: -0.020 min  
Response: 117038  
Conc: 0.83 ug/ml