

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071323\
Data File : FE043191.D
Signal(s) : FID1B.ch
Acq On : 12 Jul 2023 22:07
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 13 03:53:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE071323.M
Quant Title :
QLast Update : Thu Jul 13 03:52:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.988	1991067	16.515 ug/ml
Target Compounds			


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071323\
Data File : FE043191.D
Signal(s) : FID1B.ch
Acq On : 12 Jul 2023 22:07
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 13 03:53:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE071323.M
Quant Title :
QLast Update : Thu Jul 13 03:52:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

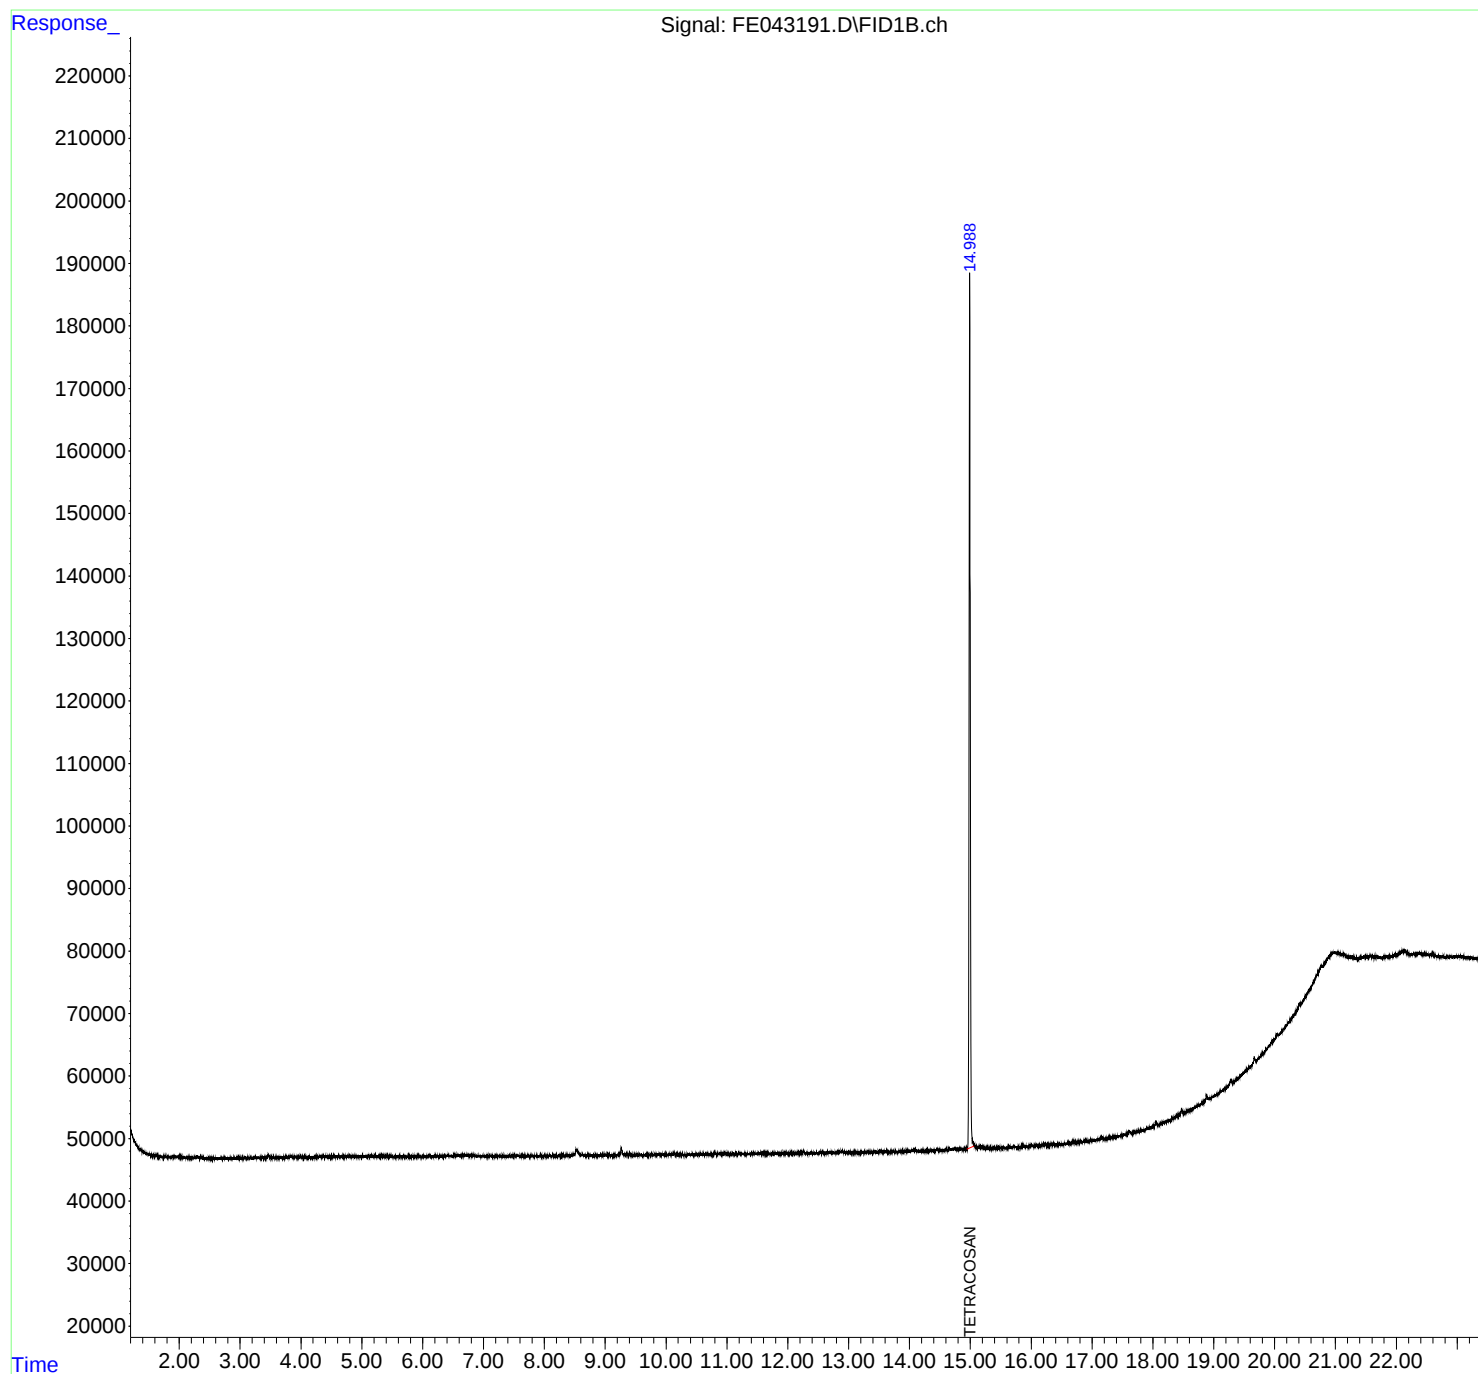

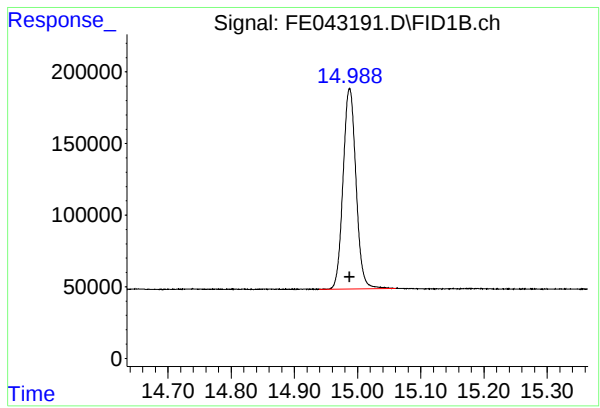

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.988 min
Delta R.T.: 0.000 min
Response: 1991067
Conc: 16.51 ug/ml