

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071421\
 Data File : FE034051.D
 Signal(s) : FID1B.CH
 Acq On : 15 Jul 2021 9:04
 Operator : DD\AJ
 Sample : M3028-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 15 13:24:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE062321.M
 Quant Title :
 QLast Update : Thu Jun 24 03:12:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.685	387172	1.107 ug/ml
Target Compounds			
7) N-EICOSANE	12.654f	1175575	2.914 ug/ml
8) N-DOCOSANE	13.845f	354222	0.879 ug/ml
10) N-TETRACOSANE	14.877	545360	1.340 ug/ml
13) N-TRIACONTANE	17.753	346939	0.858 ug/ml
14) N-DOTRIACONTANE	18.580	356302	0.899 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071421\
Data File : FE034051.D
Signal(s) : FID1B.CH
Acq On : 15 Jul 2021 9:04
Operator : DD\AJ
Sample : M3028-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 15 13:24:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE062321.M
Quant Title :
QLast Update : Thu Jun 24 03:12:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

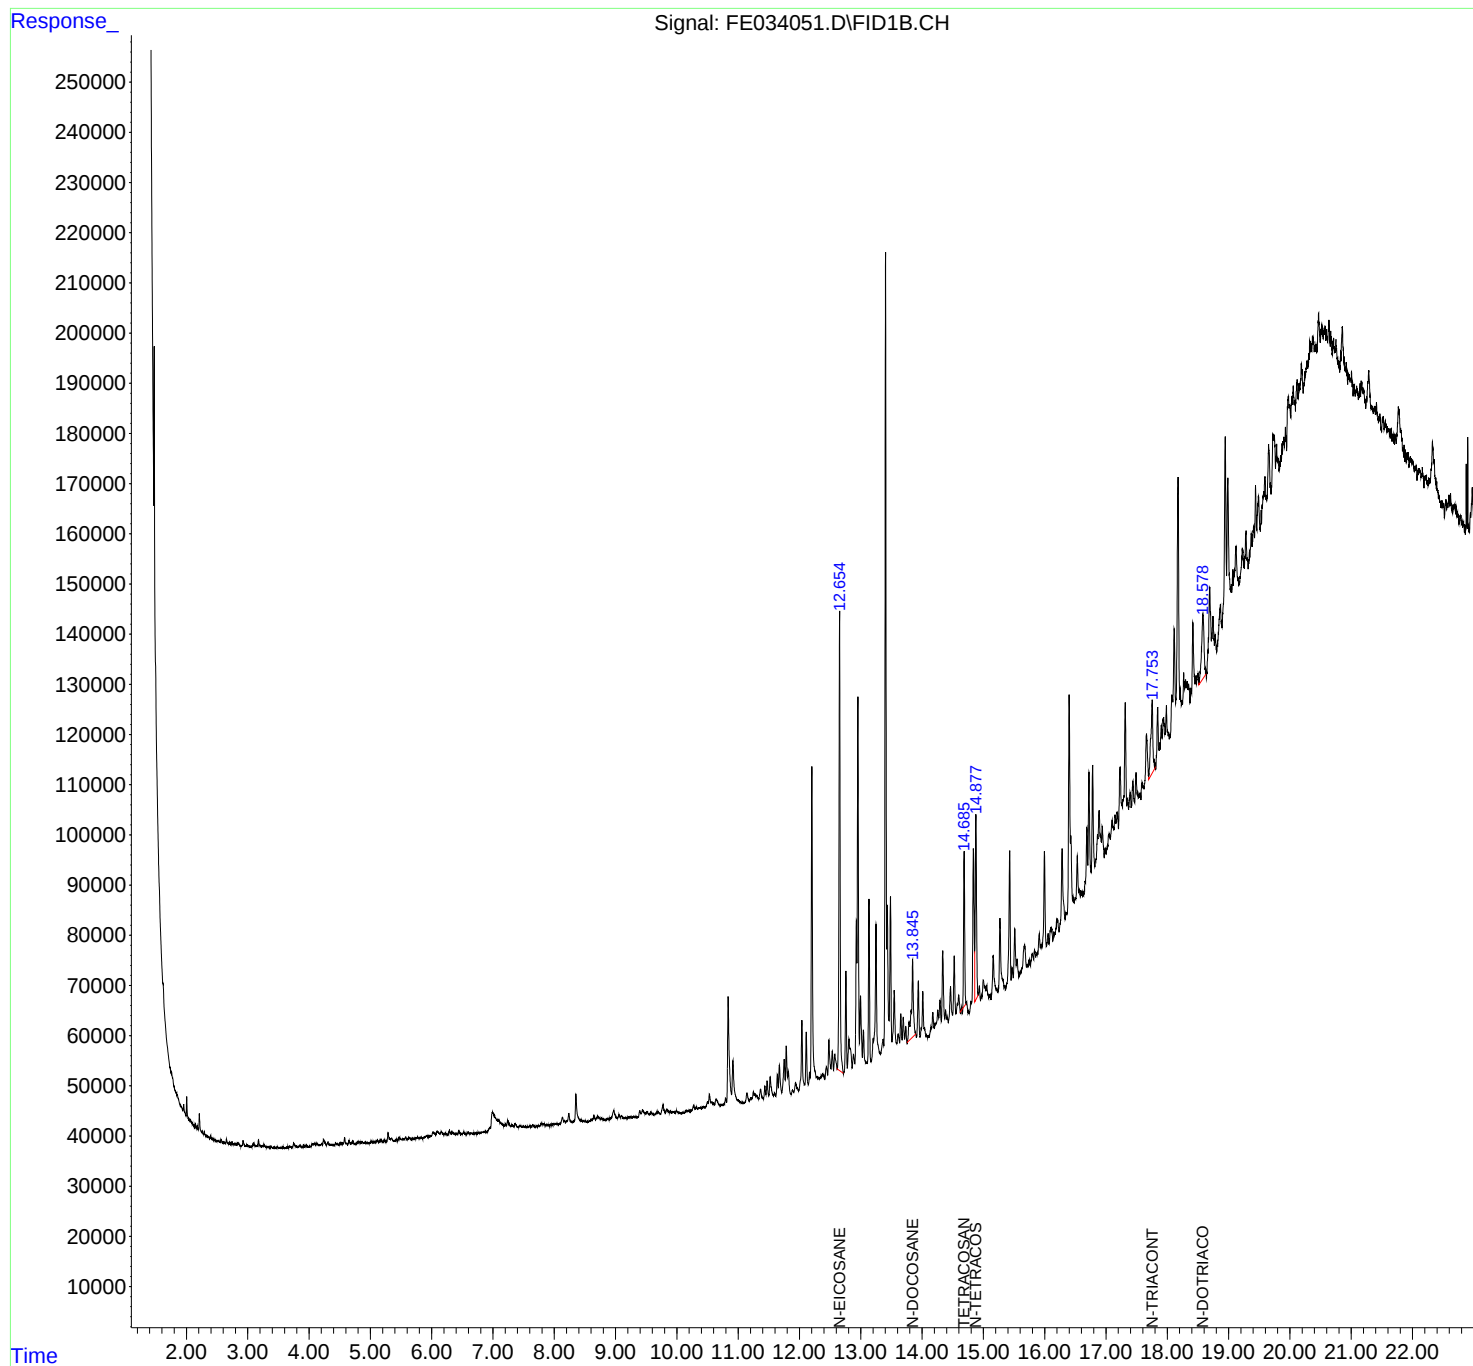


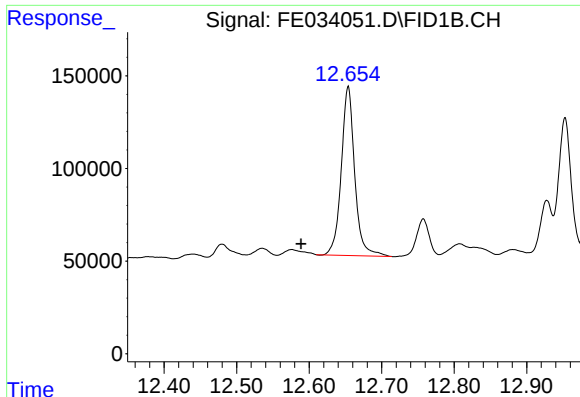

#7 N-EICOSANE


R.T.: 12.654 min
Delta R.T.: 0.065 min
Response: 1175575
Conc: 2.91 ug/ml

Instrument :
FID_E
ClientSampleId :

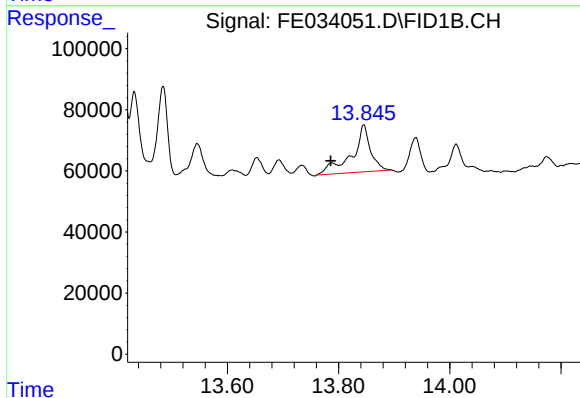


#8 N-DOCOSANE

R.T.: 13.845 min
Delta R.T.: 0.059 min
Response: 354222
Conc: 0.88 ug/ml

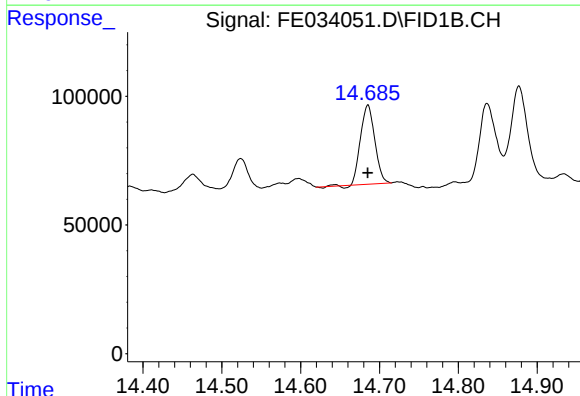


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.685 min
Delta R.T.: 0.000 min
Response: 387172
Conc: 1.11 ug/ml

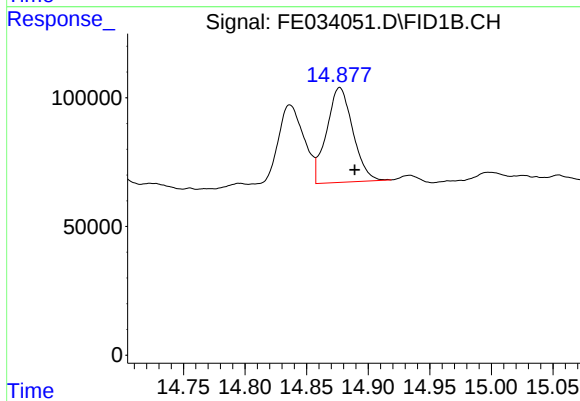

#10 N-TETRACOSANE


R.T.: 14.877 min
Delta R.T.: -0.012 min
Response: 545360
Conc: 1.34 ug/ml

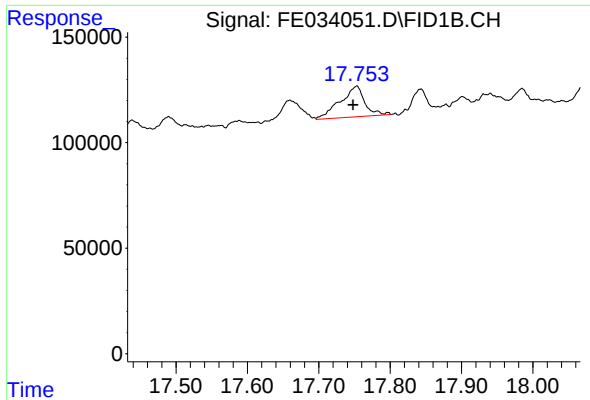

#13 N-TRIACONTANE

R.T.: 17.753 min
Delta R.T.: 0.005 min
Response: 346939
Conc: 0.86 ug/ml

Instrument :
FID_E
ClientSampleId :

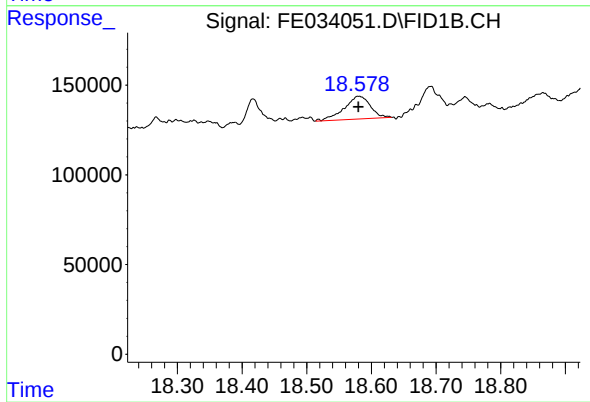

#14 N-DOTRIACONTANE

R.T.: 18.580 min
Delta R.T.: 0.000 min
Response: 356302
Conc: 0.90 ug/ml