

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071621\
Data File : FE034079.D
Signal(s) : FID1B.CH
Acq On : 16 Jul 2021 15:26
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 17 00:52:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE062321.M
Quant Title :
QLast Update : Thu Jun 24 03:12:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.683	7022828	20.075 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071621\
Data File : FE034079.D
Signal(s) : FID1B.CH
Acq On : 16 Jul 2021 15:26
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 17 00:52:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE062321.M
Quant Title :
QLast Update : Thu Jun 24 03:12:19 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

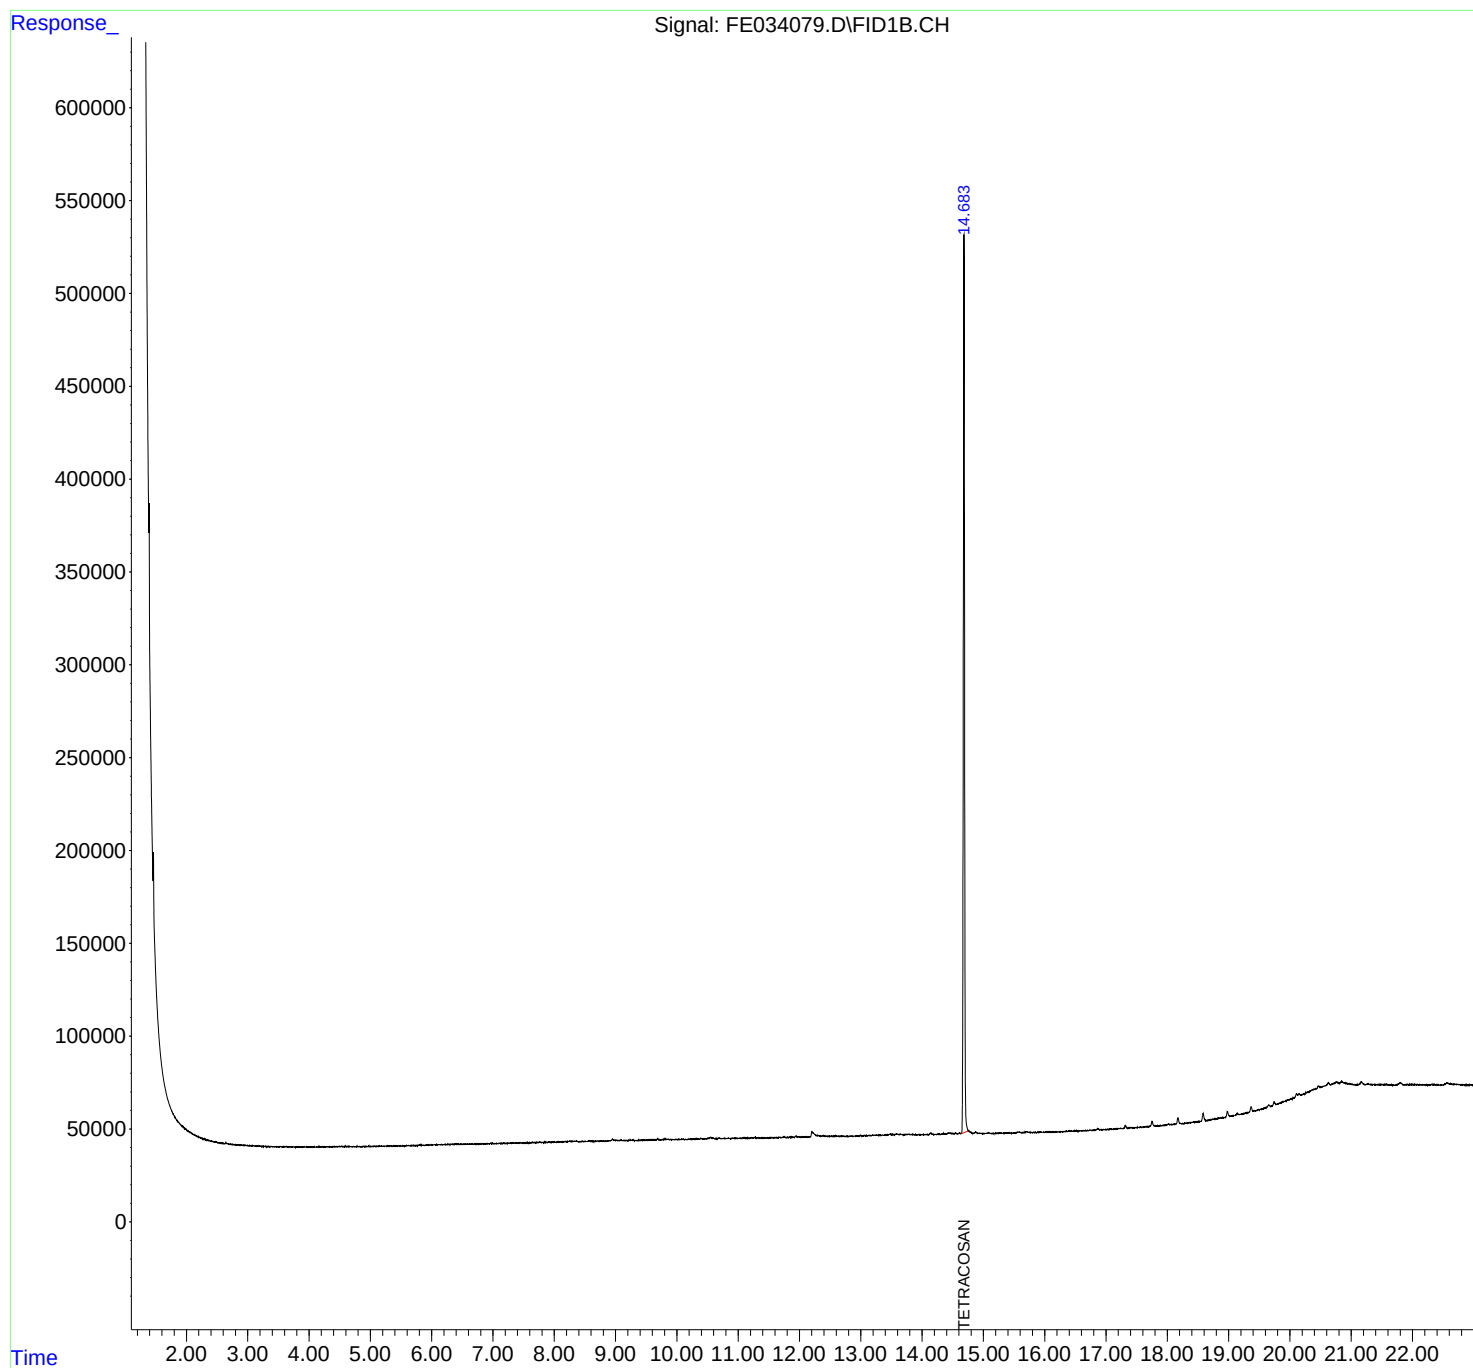

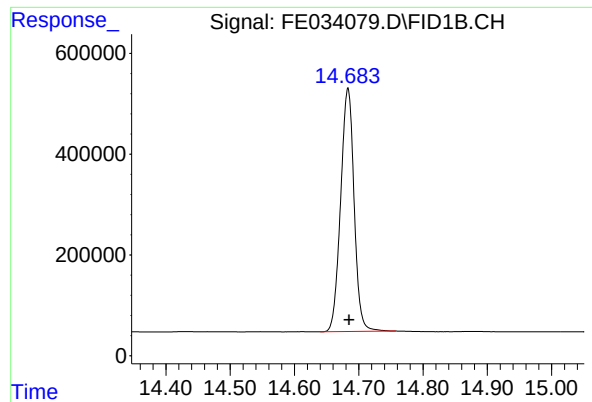

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.683 min
Delta R.T.: -0.002 min
Response: 7022828
Conc: 20.08 ug/ml

Instrument :
FID_E
ClientSampleId :