

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE071625AL\  
 Data File : FE054869.D  
 Signal(s) : FID1B.ch  
 Acq On : 16 Jul 2025 08:20  
 Operator : YP\AJ  
 Sample : Q2595-02DL 5X  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 CHRT-24849-E2DL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 07/17/2025  
 Supervised By :mohammad ahmed 07/18/2025

Integration File: autoint1.e  
 Quant Time: Jul 16 12:26:32 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 062725.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Jul 08 07:45:12 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 12.083 | 785920     | 4.840 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 9.68%        |
| 12) S 1-chlorooctadecane (S... | 13.520 | 636474     | 5.040 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 10.08%       |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE071625AL\  
Data File : FE054869.D  
Signal(s) : FID1B.ch  
Acq On : 16 Jul 2025 08:20  
Operator : YP\AJ  
Sample : Q2595-02DL 5X  
Misc :  
ALS Vial : 12 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
CHRT-24849-E2DL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 07/17/2025  
Supervised By :mohammad ahmed 07/18/2025

Integration File: autoint1.e  
Quant Time: Jul 16 12:26:32 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 062725.M  
Quant Title : GC Extractables  
QLast Update : Tue Jul 08 07:45:12 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

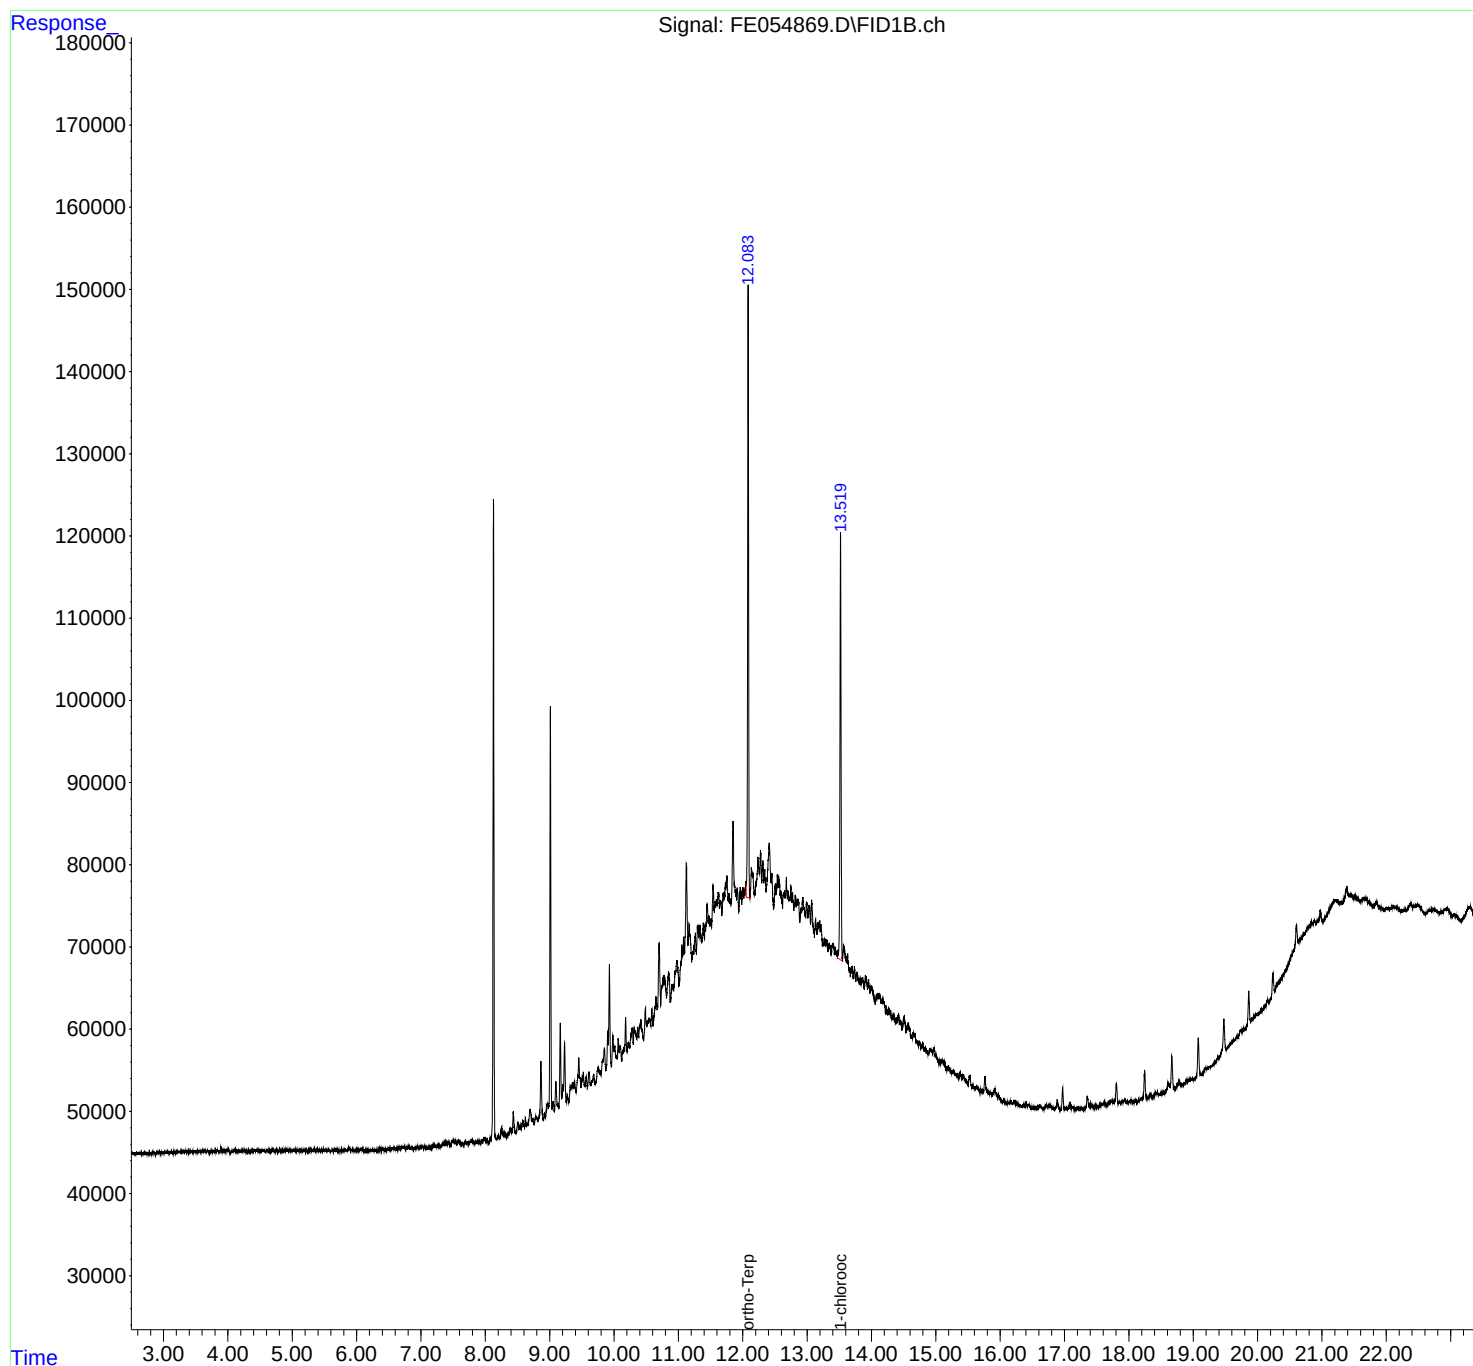

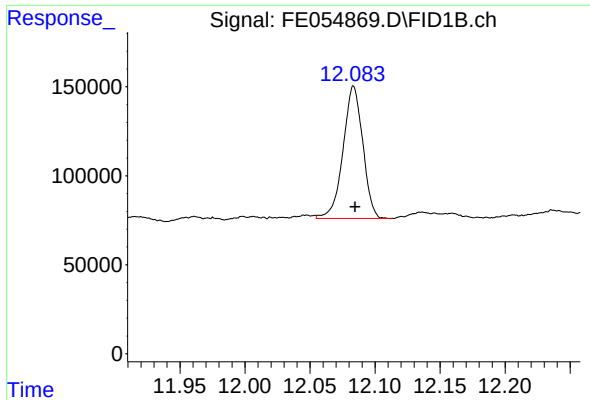

#9 ortho-Terphenyl (SURR)

R.T.: 12.083 min  
Delta R.T.: -0.002 min  
Response: 785920  
Conc: 4.84 ug/ml

Instrument :

FID\_E

ClientSampleId :


CHRT-24849-E2DL

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/17/2025

Supervised By :mohammad ahmed 07/18/2025

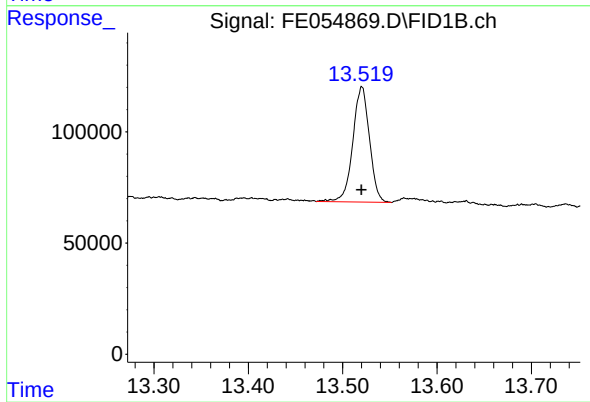

#12 1-chlorooctadecane (SURR)

R.T.: 13.520 min  
Delta R.T.: 0.000 min  
Response: 636474  
Conc: 5.04 ug/ml