

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071720\
 Data File : FE032393.D
 Signal(s) : FID1B.CH
 Acq On : 17 Jul 2020 12:40
 Operator : DD\AJ
 Sample : L3276-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 WASTE

Integration File: autoint1.e
 Quant Time: Jul 18 00:21:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE070720.M
 Quant Title :
 QLast Update : Wed Jul 08 12:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.742	7974251	26.212 ug/ml
Target Compounds			
4) N-TETRADECANE	8.356	2697716	7.763 ug/ml
7) N-EICOSANE	12.713	262505	0.746 ug/ml
10) N-TETRACOSANE	14.989	235395	0.665 ug/ml
12) N-OCTACOSANE	16.909	377904	1.075 ug/ml
13) N-TRIACONTANE	17.796	524192	1.491 ug/ml
14) N-DOTRIACONTANE	18.624	605107	1.819 ug/ml
15) N-TETRATRIACONTANE	19.410	194151	0.692 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071720\
Data File : FE032393.D
Signal(s) : FID1B.CH
Acq On : 17 Jul 2020 12:40
Operator : DD\AJ
Sample : L3276-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
WASTE

Integration File: autoint1.e
Quant Time: Jul 18 00:21:46 2020
Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE070720.M
Quant Title :
QLast Update : Wed Jul 08 12:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

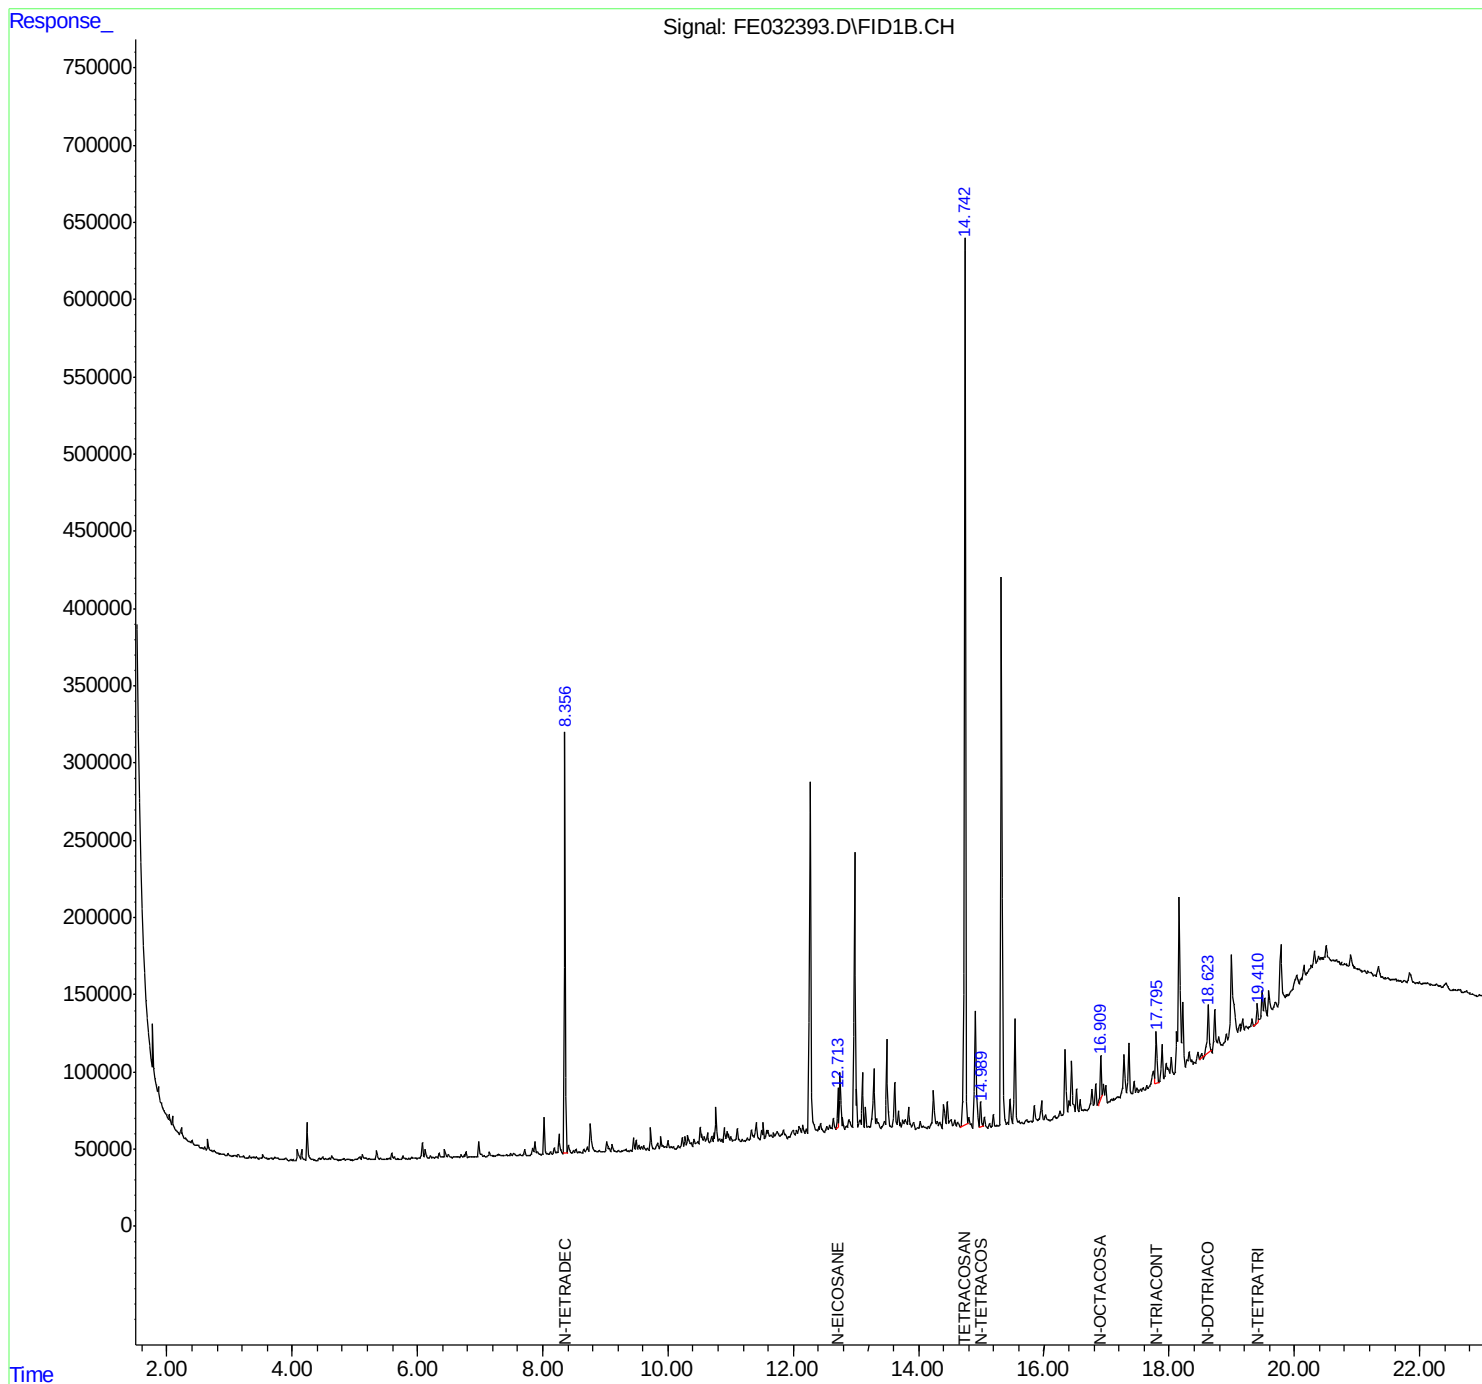


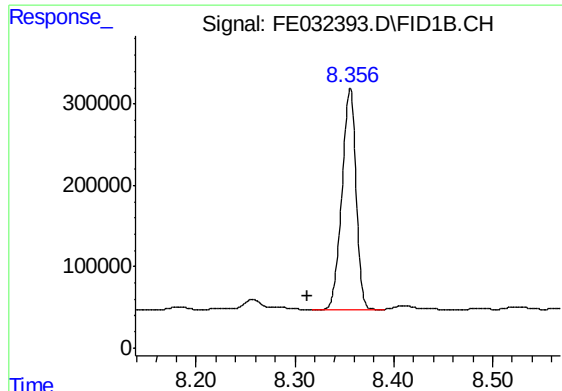

#4 N-TETRADECANE


R.T.: 8.356 min
Delta R.T.: 0.043 min
Response: 2697716
Conc: 7.76 ug/ml

Instrument :
FID_E
ClientSampleId :
WASTE

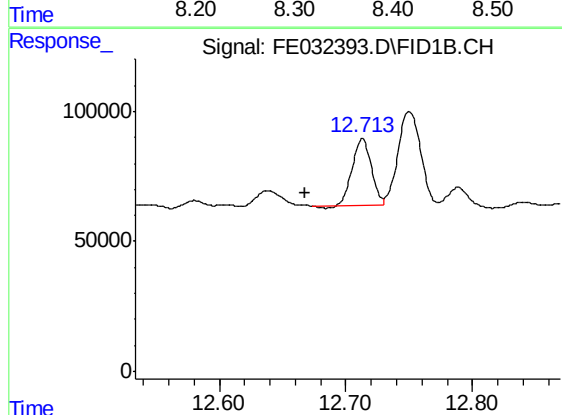


#7 N-EICOSANE

R.T.: 12.713 min
Delta R.T.: 0.045 min
Response: 262505
Conc: 0.75 ug/ml

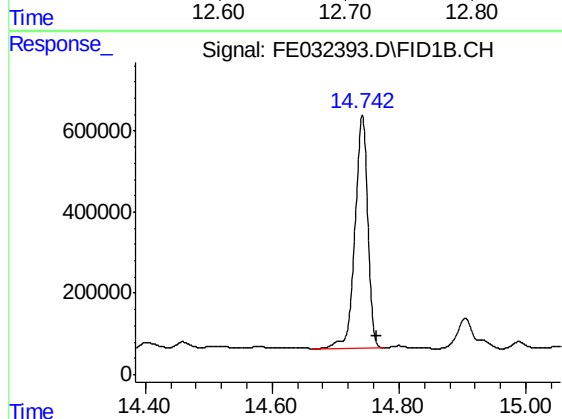


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.742 min
Delta R.T.: -0.021 min
Response: 7974251
Conc: 26.21 ug/ml

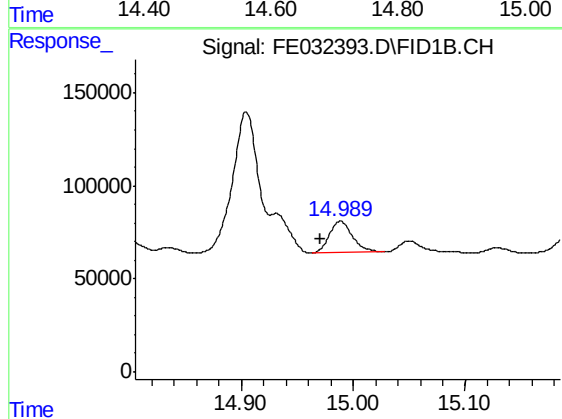

#10 N-TETRACOSANE


R.T.: 14.989 min
Delta R.T.: 0.019 min
Response: 235395
Conc: 0.66 ug/ml

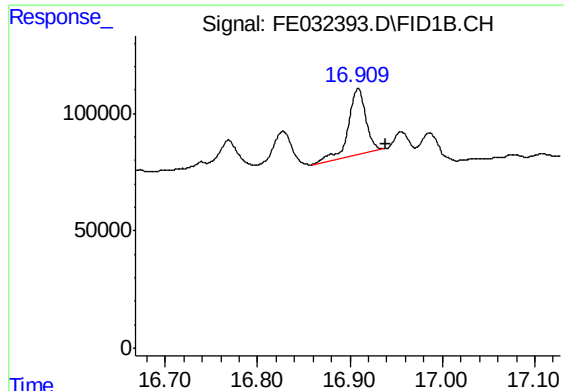

#12 N-OCTACOSANE


R.T.: 16.909 min
Delta R.T.: -0.030 min
Response: 377904
Conc: 1.07 ug/ml

Instrument :
FID_E
ClientSampleId :
WASTE

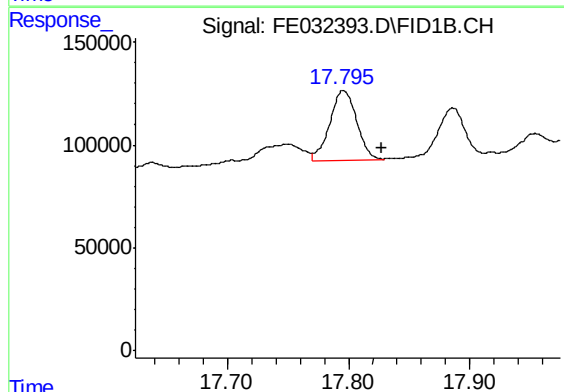


#13 N-TRIACONTANE

R.T.: 17.796 min
Delta R.T.: -0.031 min
Response: 524192
Conc: 1.49 ug/ml

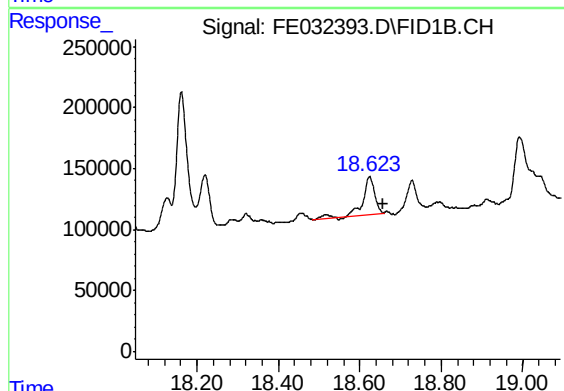

#14 N-DOTRIACONTANE

R.T.: 18.624 min
Delta R.T.: -0.033 min
Response: 605107
Conc: 1.82 ug/ml

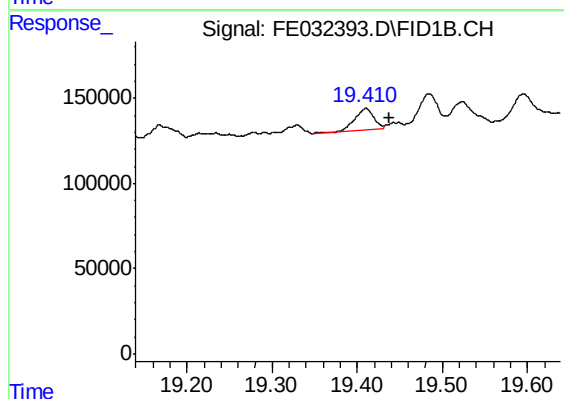

#15 N-TETRATRIACONTANE

R.T.: 19.410 min
Delta R.T.: -0.028 min
Response: 194151
Conc: 0.69 ug/ml