

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE071720\  
 Data File : FE032411.D  
 Signal(s) : FID1B.CH  
 Acq On : 17 Jul 2020 22:08  
 Operator : DD\AJ  
 Sample : L3328-07  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jul 18 00:25:26 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE070720.M  
 Quant Title :  
 QLast Update : Wed Jul 08 12:04:06 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.734	6539641	21.496 ug/ml
Target Compounds			
3) N-DODECANE	6.497	779919	2.235 ug/ml
4) N-TETRADECANE	8.280	318466	0.916 ug/ml
5) N-HEXADECANE	9.906	317663	0.911 ug/ml
13) N-TRIACONTANE	17.785	213823	0.608 ug/ml
14) N-DOTRIACONTANE	18.616	243016	0.730 ug/ml
16) N-HEXATRIACONTANE	20.138	163796	0.758 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE071720\  
 Data File : FE032411.D  
 Signal(s) : FID1B.CH  
 Acq On : 17 Jul 2020 22:08  
 Operator : DD\AJ  
 Sample : L3328-07  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Jul 18 00:25:26 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE070720.M  
 Quant Title :  
 QLast Update : Wed Jul 08 12:04:06 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

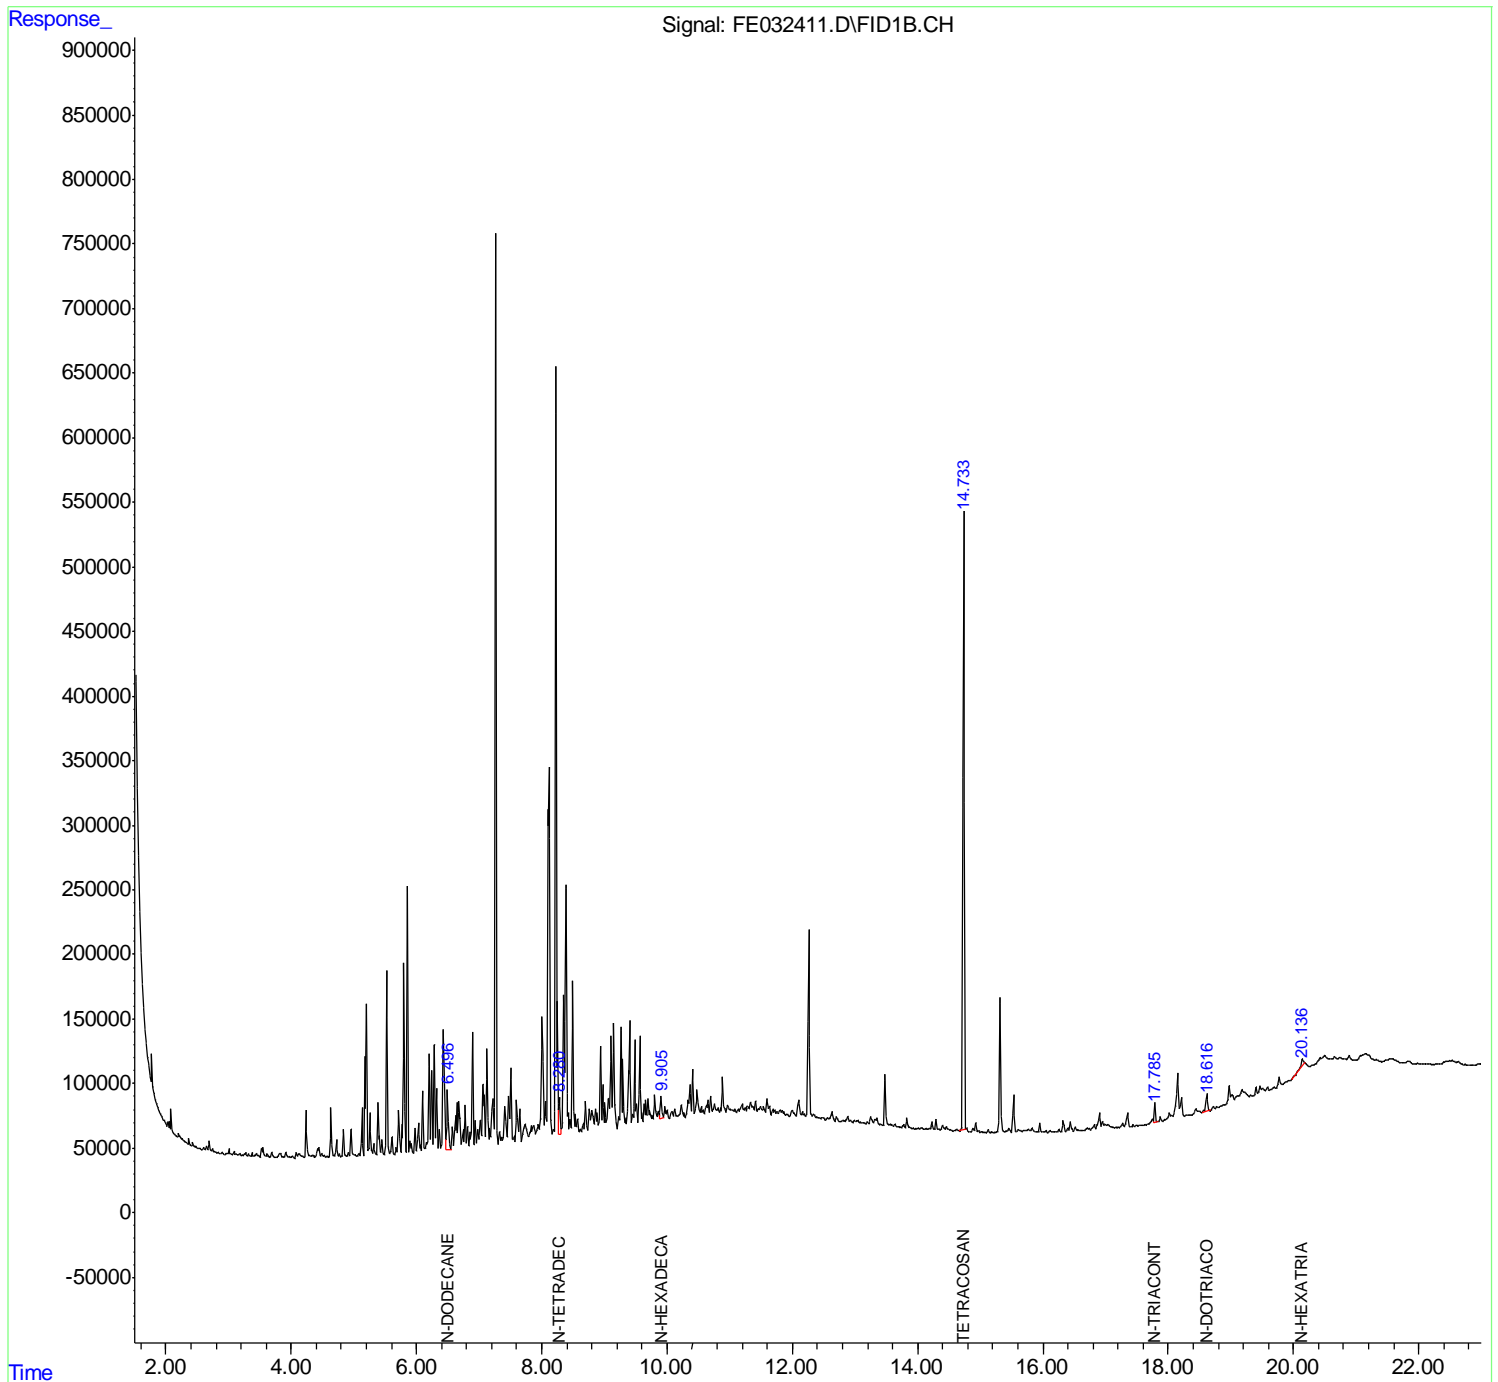


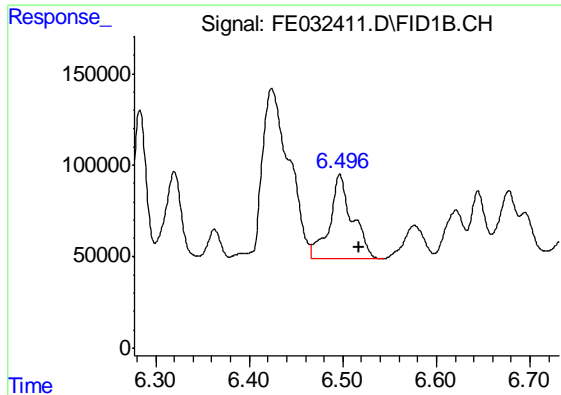

#3 N-DODECANE


R.T.: 6.497 min  
 Delta R.T.: -0.021 min  
 Response: 779919  
 Conc: 2.23 ug/ml

Instrument :  
 FID\_E  
 ClientSampled :

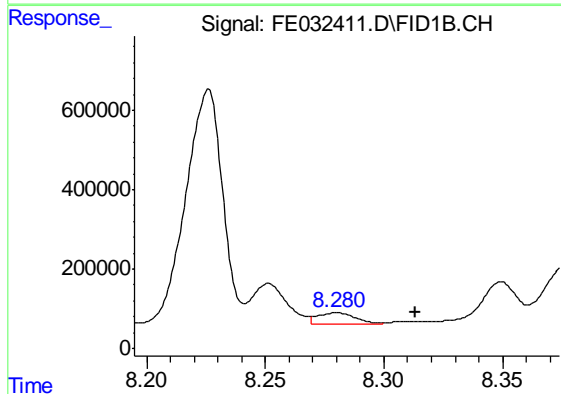


#4 N-TETRADECANE

R.T.: 8.280 min  
 Delta R.T.: -0.033 min  
 Response: 318466  
 Conc: 0.92 ug/ml

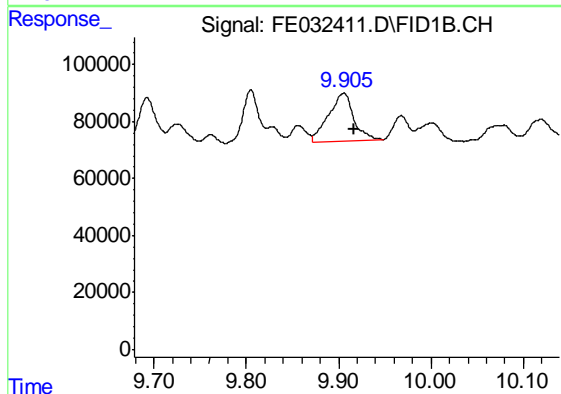


#5 N-HEXADECANE

R.T.: 9.906 min  
 Delta R.T.: -0.011 min  
 Response: 317663  
 Conc: 0.91 ug/ml

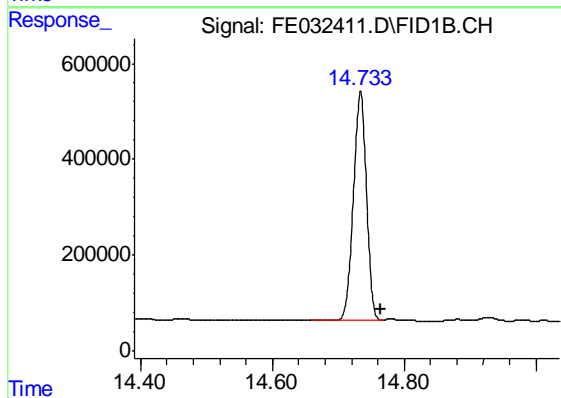

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.734 min  
 Delta R.T.: -0.030 min  
 Response: 6539641  
 Conc: 21.50 ug/ml

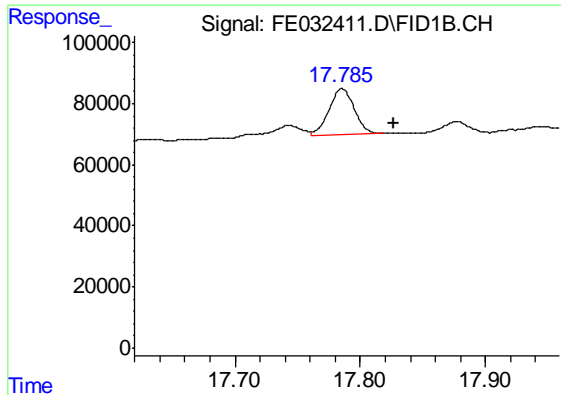

#13 N-TRIACONTANE


R.T.: 17.785 min  
Delta R.T.: -0.042 min  
Response: 213823  
Conc: 0.61 ug/ml

Instrument :  
FID\_E  
ClientSampleId :

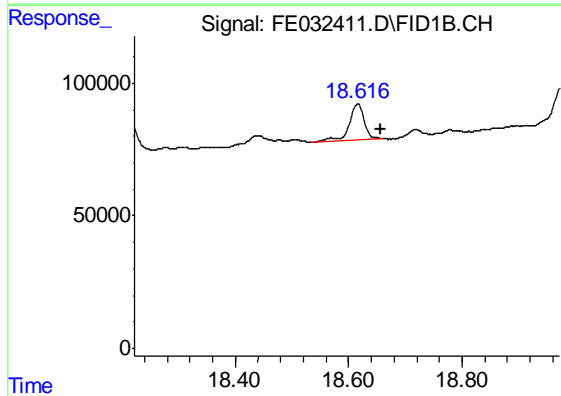

#14 N-DOTRIACONTANE

R.T.: 18.616 min  
Delta R.T.: -0.041 min  
Response: 243016  
Conc: 0.73 ug/ml

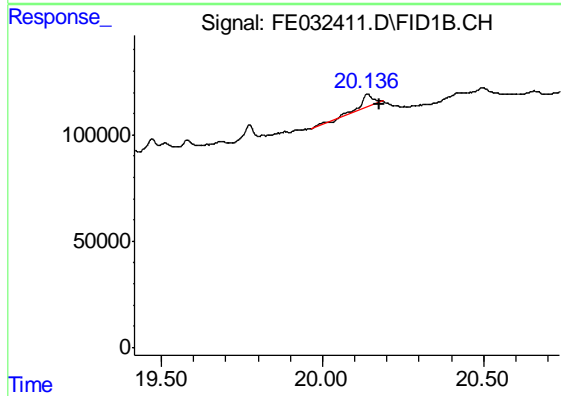

#16 N-HEXATRIACONTANE

R.T.: 20.138 min  
Delta R.T.: -0.037 min  
Response: 163796  
Conc: 0.76 ug/ml