

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071823AL\
 Data File : FE043278.D
 Signal(s) : FID1B.ch
 Acq On : 18 Jul 2023 06:16
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 19 01:48:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071323.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 13 03:02:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
11) T n-Heneicosane (C21)	13.534	231220	1.526 ug/ml
18) T n-Dotriacontane (C32)	18.879	119101	0.804 ug/ml
20) T n-Hexatriacontane (C36)	20.407	72806	0.495 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071823AL\
Data File : FE043278.D
Signal(s) : FID1B.ch
Acq On : 18 Jul 2023 06:16
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 19 01:48:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071323.M
Quant Title : GC Extractables
QLast Update : Thu Jul 13 03:02:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

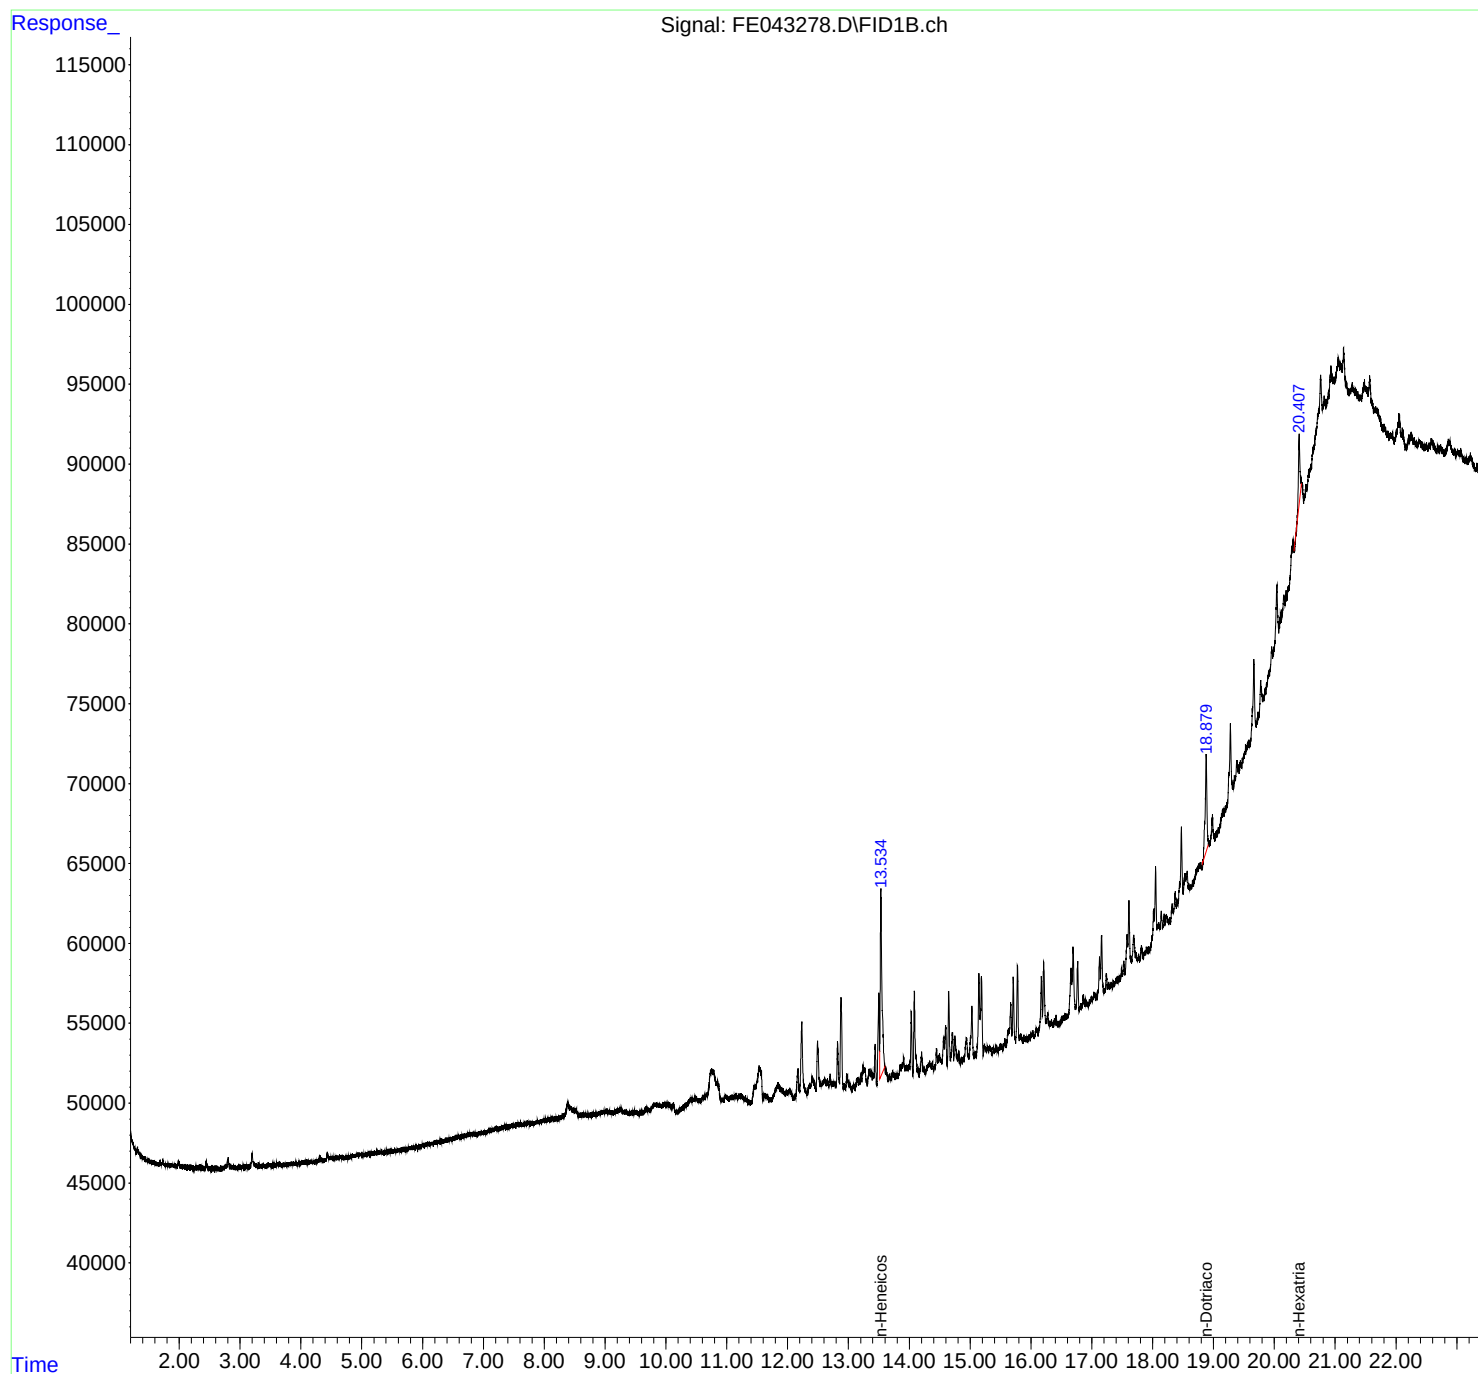


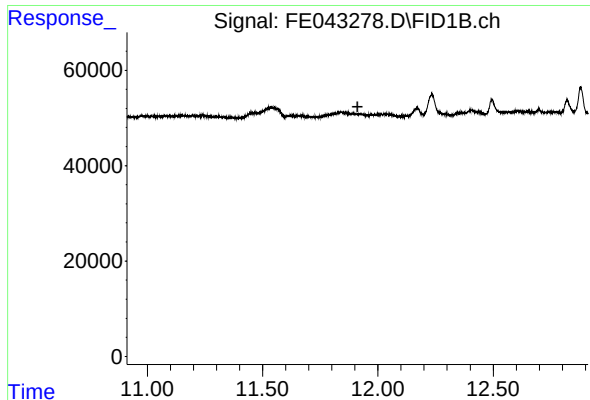

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.911 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

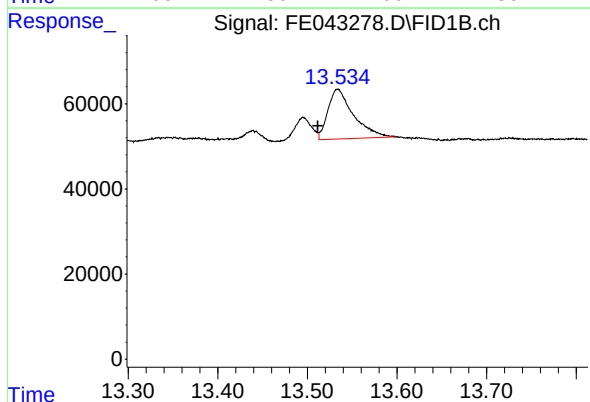


#11 n-Heneicosane (C21)

R.T.: 13.534 min
Delta R.T.: 0.022 min
Response: 231220
Conc: 1.53 ug/ml

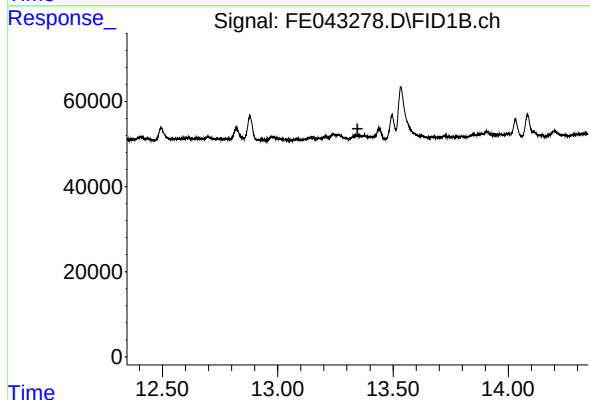


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.346 min
Response: 0
Conc: N.D.

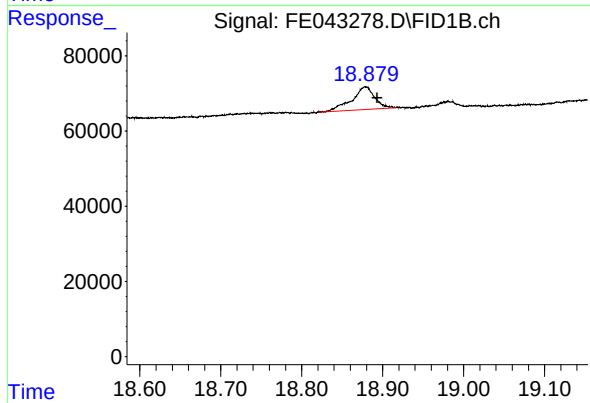

#18 n-Dotriacontane (C32)

R.T.: 18.879 min
Delta R.T.: -0.015 min
Response: 119101
Conc: 0.80 ug/ml

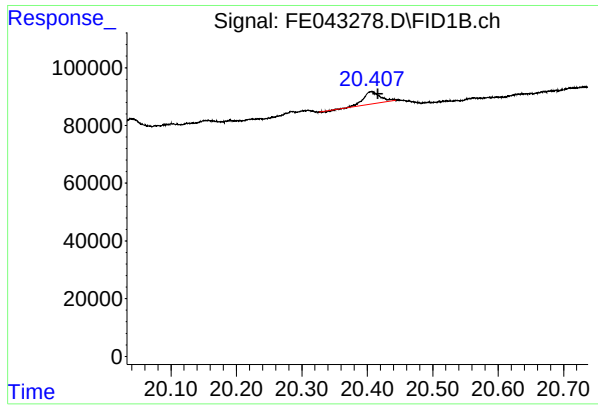

#20 n-Hexatriacontane (C36)

R.T.: 20.407 min
Delta R.T.: -0.010 min
Response: 72806
Conc: 0.50 ug/ml

Instrument :

FID_E

ClientSampleId :