

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071824AL\
 Data File : FE049178.D
 Signal(s) : FID1B.ch
 Acq On : 18 Jul 2024 12:02
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 19 01:30:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071724.M
 Quant Title : GC Extractables
 QLast Update : Wed Jul 17 14:26:40 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.893	45403	0.314 ug/ml
11) T	n-Heneicosane (C21)	13.508	26439	0.186 ug/ml
14) T	n-Tetracosane (C24)	15.155	31103	0.222 ug/ml
15) T	n-Hexacosane (C26)	16.233	69555	0.496 ug/ml
18) T	n-Dotriacontane (C32)	18.886	127311	0.866 ug/ml
19) T	n-Tetratriacontane (C34)	19.665	79040	0.541 ug/ml
20) T	n-Hexatriacontane (C36)	20.409	71804	0.498 ug/ml
21) T	n-Octatriacontane (C38)	21.139	87598	0.585 ug/ml
22) T	n-Tetracontane (C40)	22.042	52632	0.349 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE071824AL\
Data File : FE049178.D
Signal(s) : FID1B.ch
Acq On : 18 Jul 2024 12:02
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 19 01:30:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071724.M
Quant Title : GC Extractables
QLast Update : Wed Jul 17 14:26:40 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

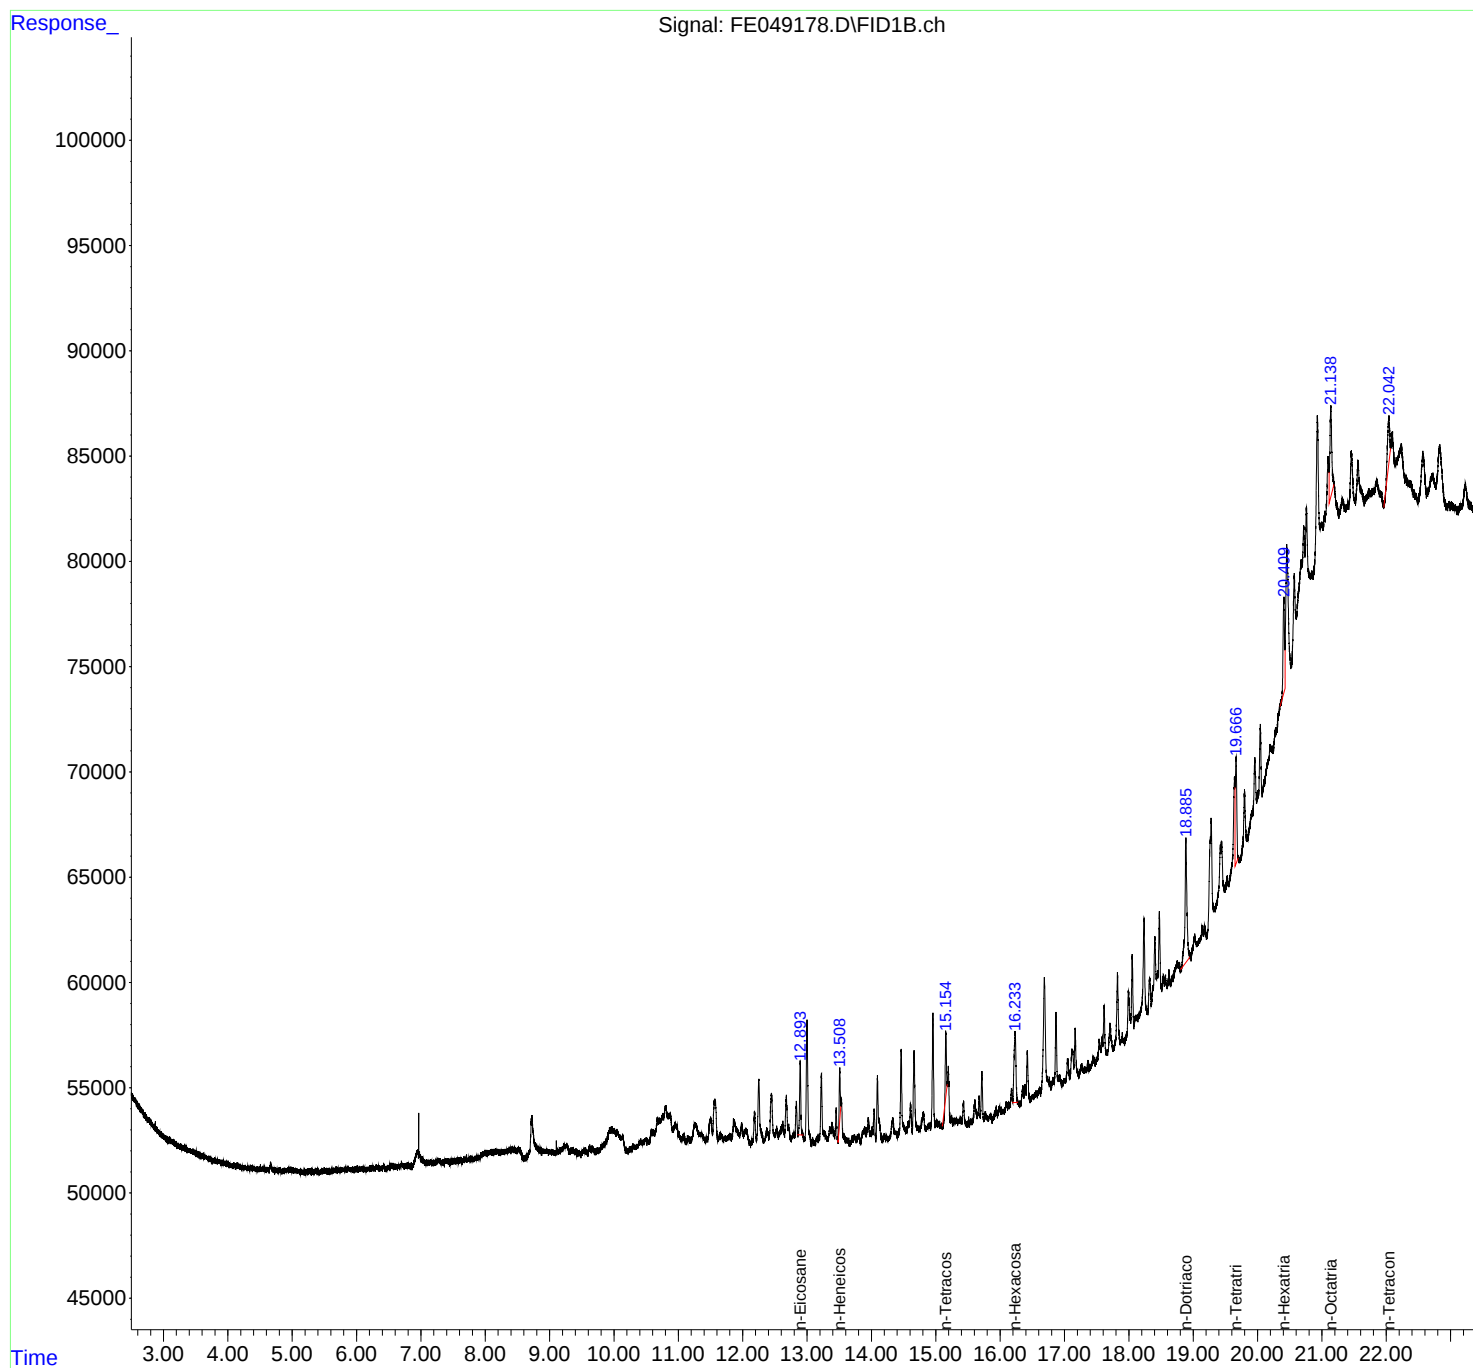


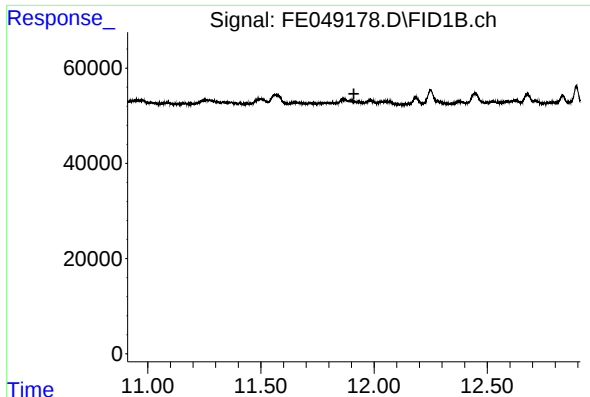

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.911 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

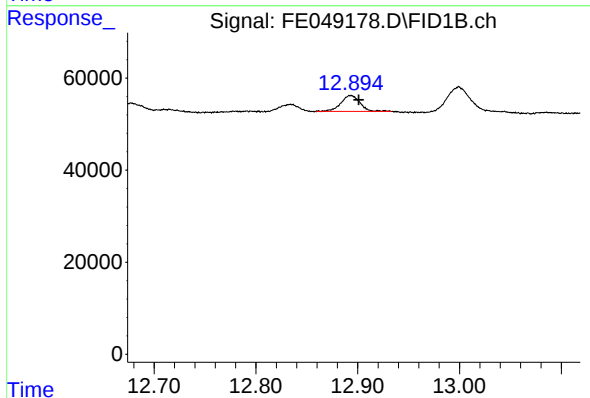


#10 n-Eicosane (C20)

R.T.: 12.893 min
Delta R.T.: -0.008 min
Response: 45403
Conc: 0.31 ug/ml

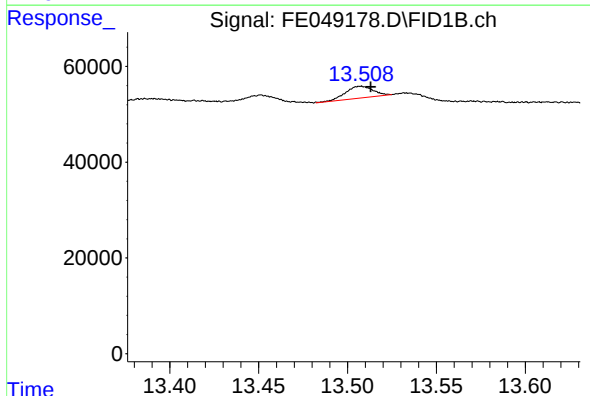


#11 n-Heneicosane (C21)

R.T.: 13.508 min
Delta R.T.: -0.006 min
Response: 26439
Conc: 0.19 ug/ml

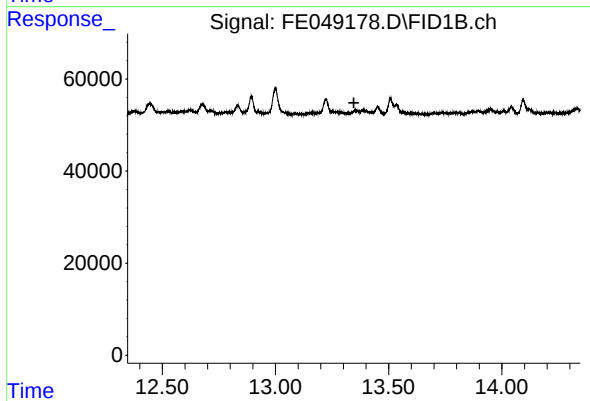

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.346 min
Response: 0
Conc: N.D.

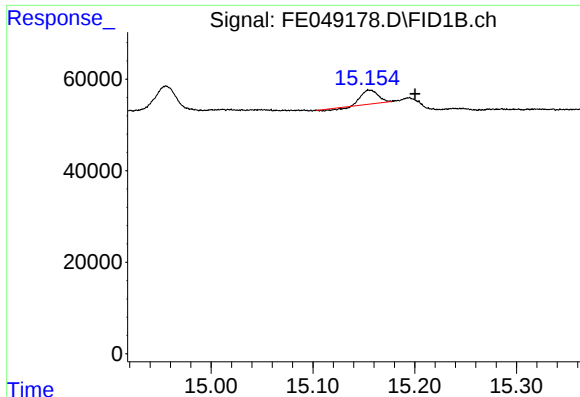

#14 n-Tetracosane (C24)


R.T.: 15.155 min
Delta R.T.: -0.045 min
Response: 31103
Conc: 0.22 ug/ml

Instrument :
FID_E
ClientSampleId :

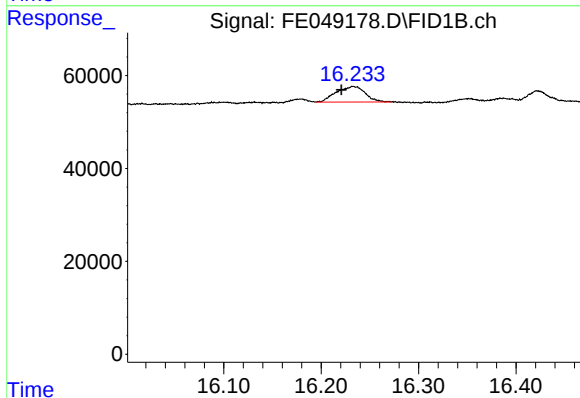


#15 n-Hexacosane (C26)

R.T.: 16.233 min
Delta R.T.: 0.012 min
Response: 69555
Conc: 0.50 ug/ml

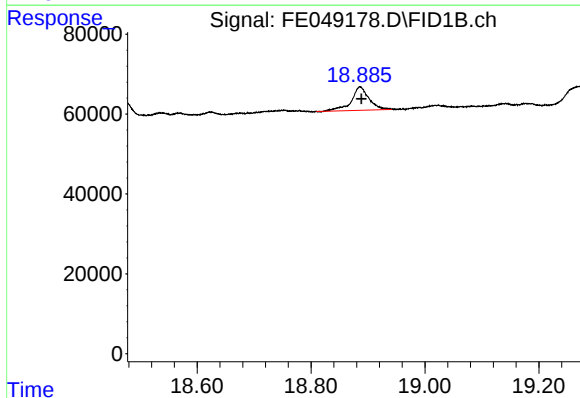


#18 n-Dotriacontane (C32)

R.T.: 18.886 min
Delta R.T.: -0.002 min
Response: 127311
Conc: 0.87 ug/ml

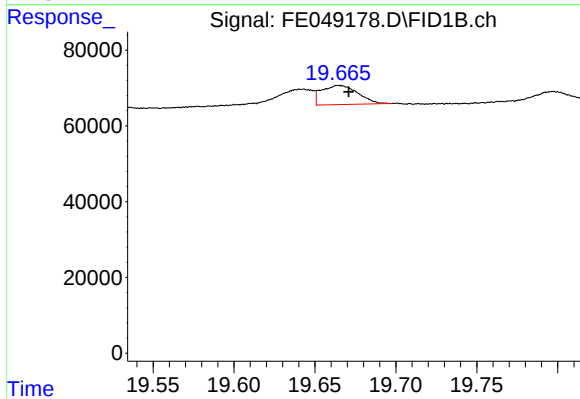

#19 n-Tetratriacontane (C34)


R.T.: 19.665 min
Delta R.T.: -0.006 min
Response: 79040
Conc: 0.54 ug/ml

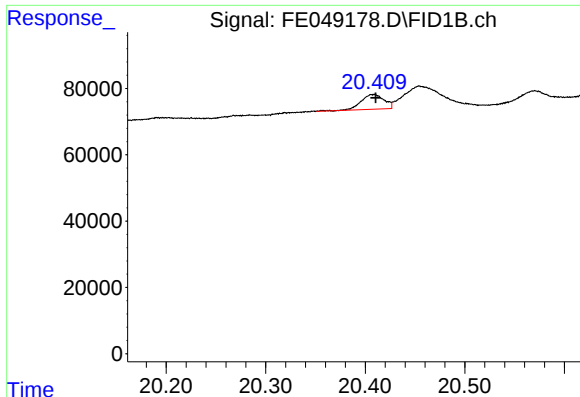

#20 n-Hexatriacontane (C36)


R.T.: 20.409 min
Delta R.T.: -0.001 min
Response: 71804
Conc: 0.50 ug/ml

Instrument :
FID_E
ClientSampleId :

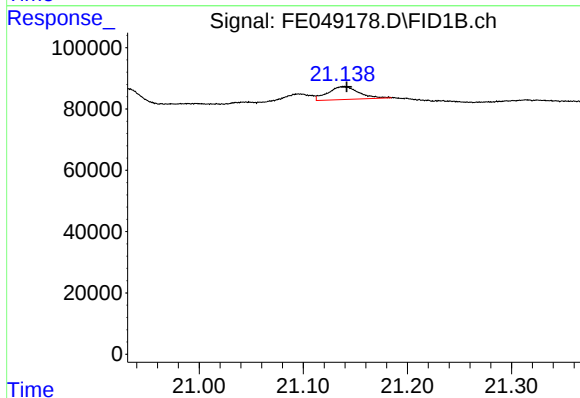

#21 n-Octatriacontane (C38)

R.T.: 21.139 min
Delta R.T.: -0.003 min
Response: 87598
Conc: 0.59 ug/ml

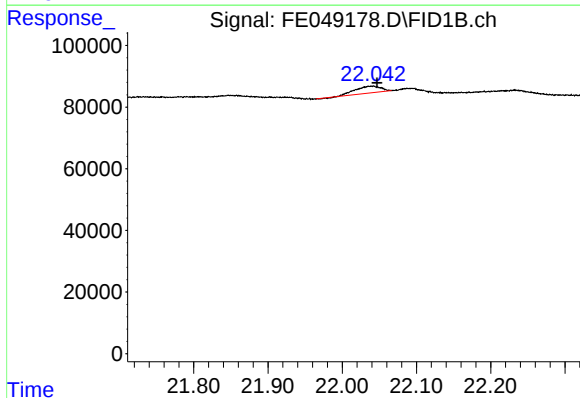

#22 n-Tetracontane (C40)

R.T.: 22.042 min
Delta R.T.: -0.005 min
Response: 52632
Conc: 0.35 ug/ml