

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072020\
 Data File : FE032417.D
 Signal(s) : FID1B.CH
 Acq On : 20 Jul 2020 13:54
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 21 02:10:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE070720.M
 Quant Title :
 QLast Update : Wed Jul 08 12:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.745	15938198	52.390 ug/ml
Target Compounds				
2)	N-DECANE	4.486	18749745	53.913 ug/ml
3)	N-DODECANE	6.503	18888480	54.125 ug/ml
4)	N-TETRADECANE	8.298	18775991	54.030 ug/ml
5)	N-HEXADECANE	9.899	18798276	53.918 ug/ml
6)	N-OCTADECANE	11.341	19006527	53.748 ug/ml
7)	N-EICOSANE	12.651	18758314	53.337 ug/ml
8)	N-DOCOSANE	13.848	18500185	52.649 ug/ml
10)	N-TETRACOSANE	14.952	18320523	51.756 ug/ml
11)	N-HEXACOSANE	15.971	17773022	50.648 ug/ml
12)	N-OCTACOSANE	16.920	17517565	49.808 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072020\
Data File : FE032417.D
Signal(s) : FID1B.CH
Acq On : 20 Jul 2020 13:54
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 21 02:10:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE070720.M
Quant Title :
QLast Update : Wed Jul 08 12:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

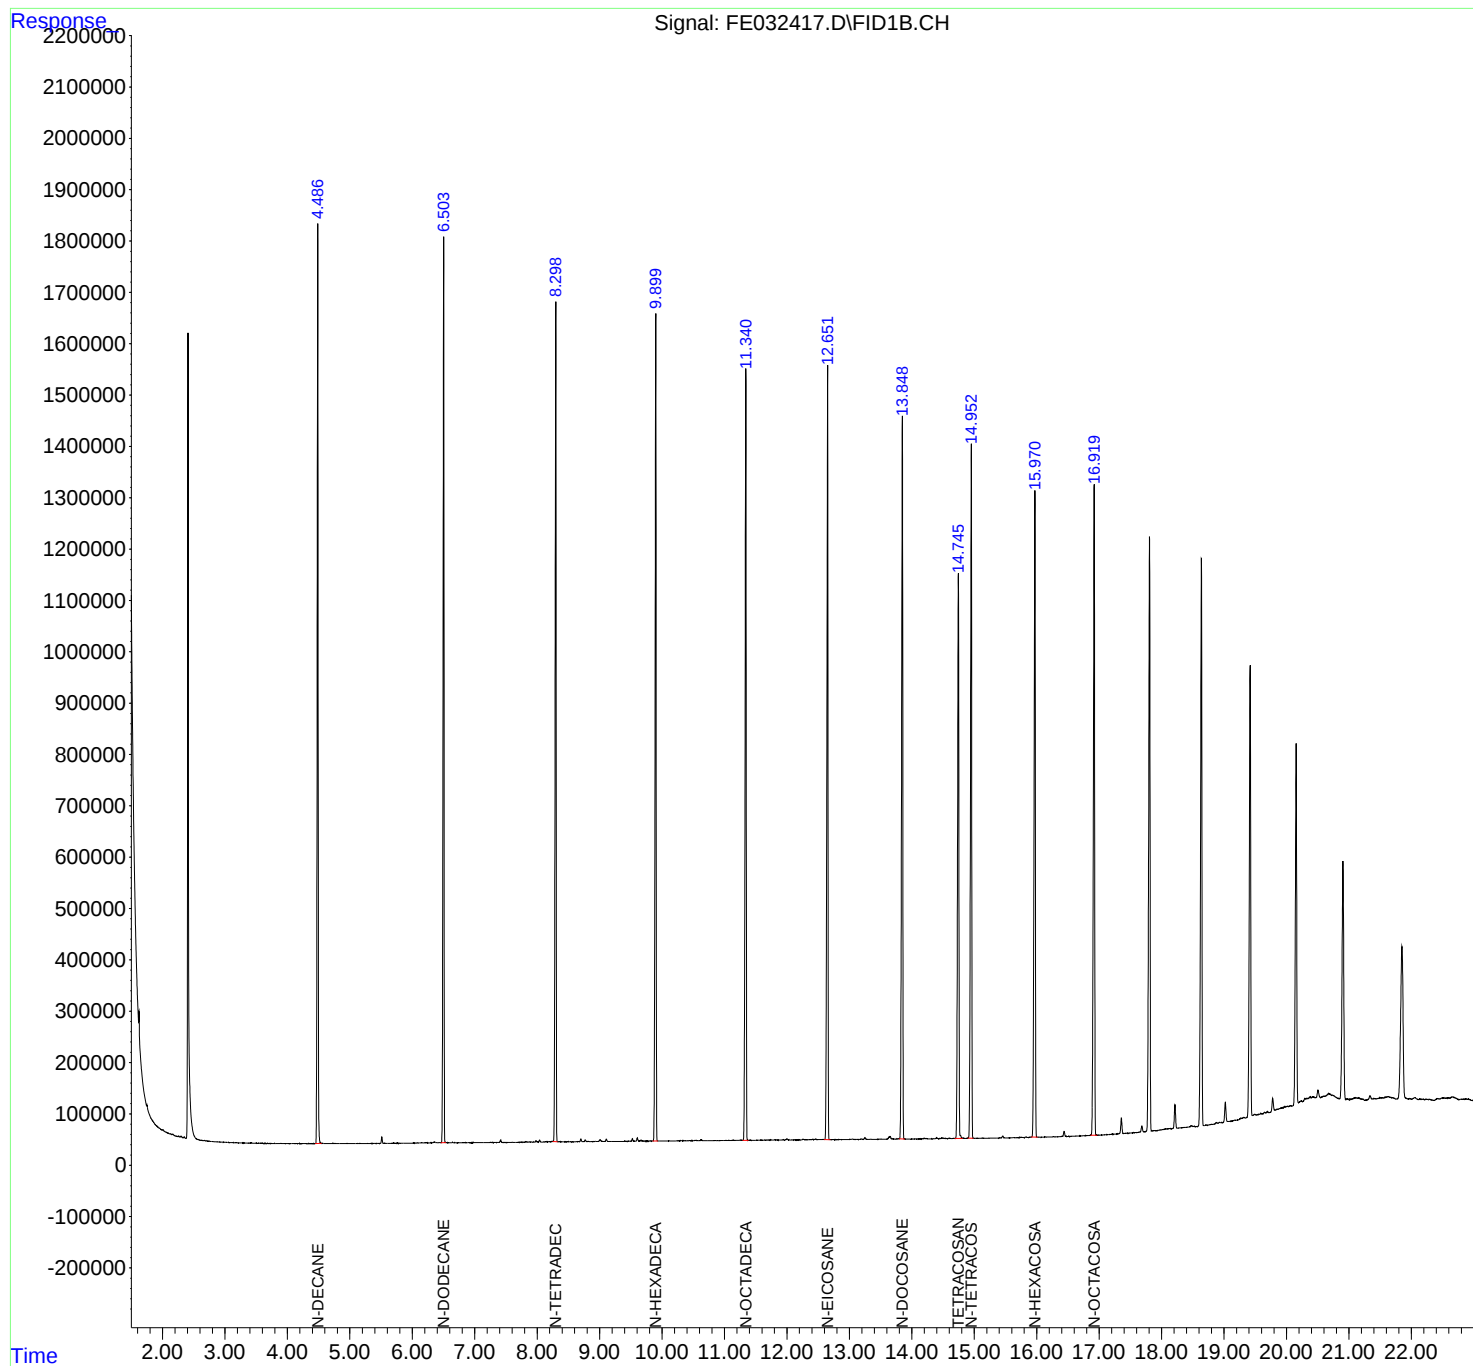

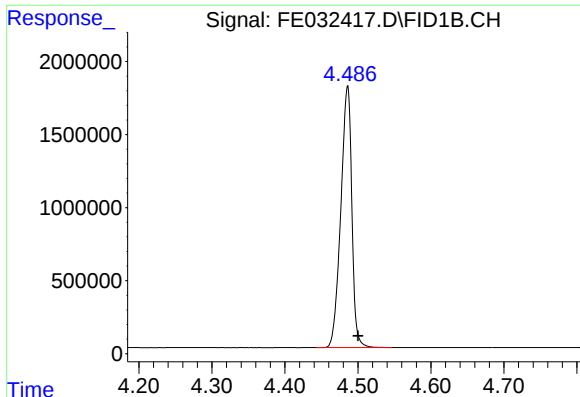


#2 N-DECANE

R.T.: 4.486 min
Delta R.T.: -0.014 min
Response: 18749745
Conc: 53.91 ug/ml

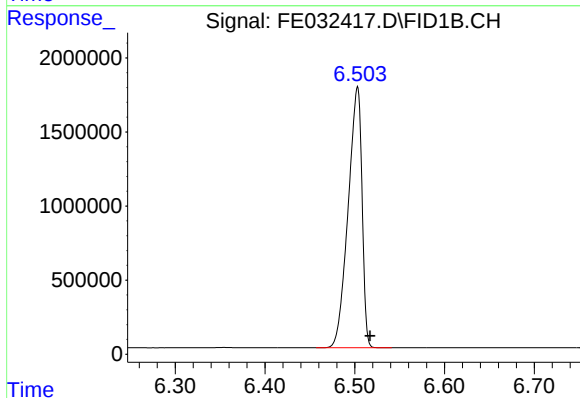


#3 N-DODECANE

R.T.: 6.503 min
Delta R.T.: -0.014 min
Response: 18888480
Conc: 54.13 ug/ml

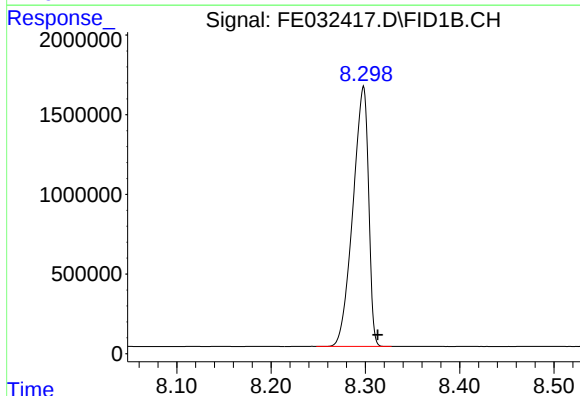


#4 N-TETRADECANE

R.T.: 8.298 min
Delta R.T.: -0.015 min
Response: 18775991
Conc: 54.03 ug/ml

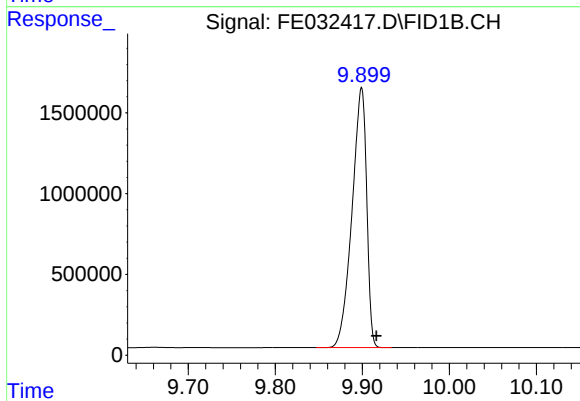


#5 N-HEXADECANE

R.T.: 9.899 min
Delta R.T.: -0.017 min
Response: 18798276
Conc: 53.92 ug/ml

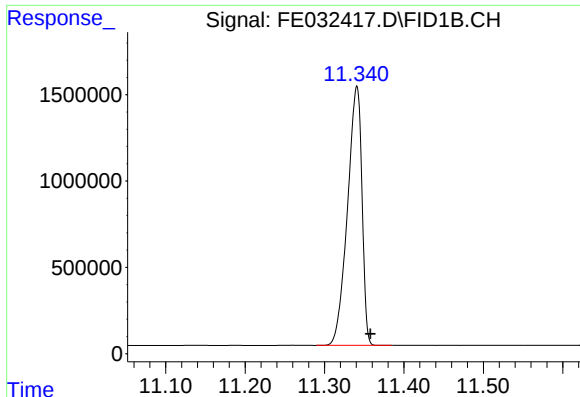


#6 N-OCTADECANE

R.T.: 11.341 min
Delta R.T.: -0.017 min
Response: 19006527
Conc: 53.75 ug/ml

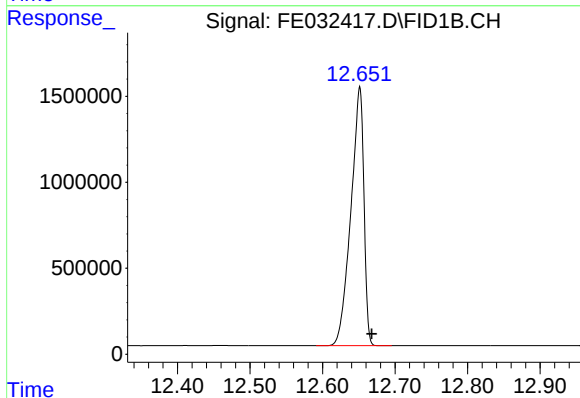


#7 N-EICOSANE

R.T.: 12.651 min
Delta R.T.: -0.017 min
Response: 18758314
Conc: 53.34 ug/ml

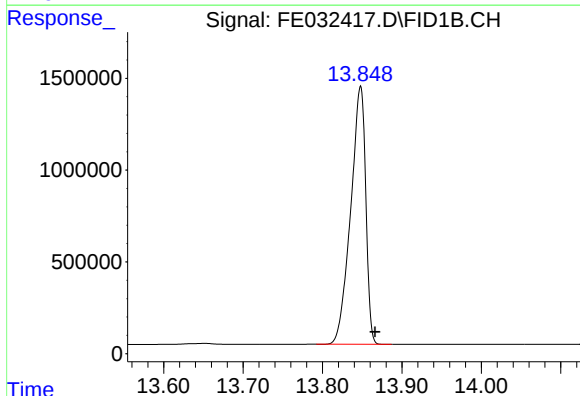


#8 N-DOCOSANE

R.T.: 13.848 min
Delta R.T.: -0.018 min
Response: 18500185
Conc: 52.65 ug/ml

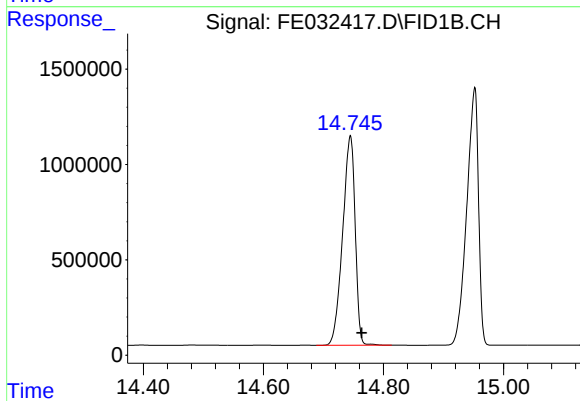


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.745 min
Delta R.T.: -0.019 min
Response: 15938198
Conc: 52.39 ug/ml

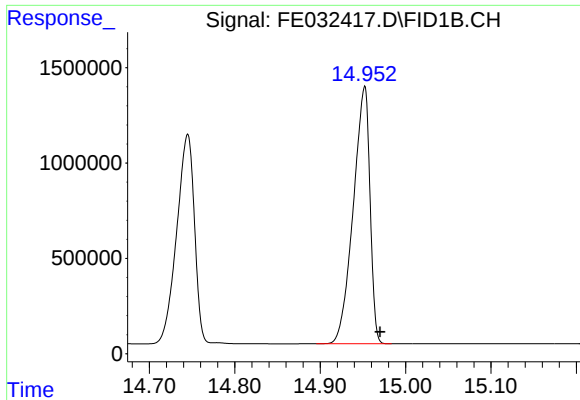


#10 N-TETRACOSANE

R.T.: 14.952 min
Delta R.T.: -0.018 min
Response: 18320523
Conc: 51.76 ug/ml

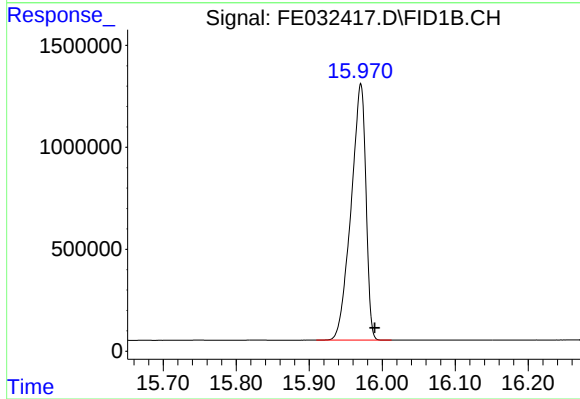

#11 N-HEXACOSANE

R.T.: 15.971 min
Delta R.T.: -0.019 min
Response: 17773022
Conc: 50.65 ug/ml

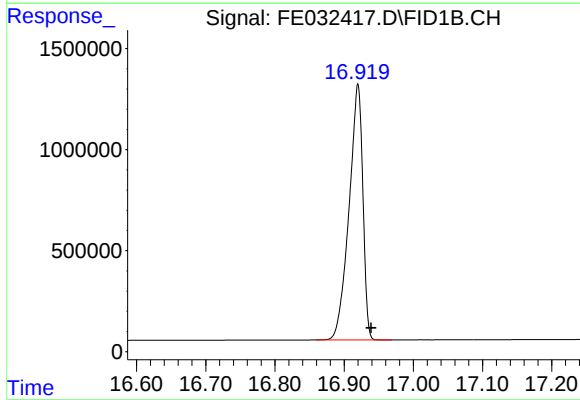

#12 N-OCTACOSANE

R.T.: 16.920 min
Delta R.T.: -0.019 min
Response: 17517565
Conc: 49.81 ug/ml