

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072220\
 Data File : FE032443.D
 Signal(s) : FID1B.CH
 Acq On : 22 Jul 2020 13:58
 Operator : DD\AJ
 Sample : PB130368BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 23 00:53:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE070720.M
 Quant Title :
 QLast Update : Wed Jul 08 12:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.743	7557493	24.842 ug/ml
Target Compounds				
2)	N-DECANE	4.485	9672222	27.812 ug/ml
3)	N-DODECANE	6.499	9682784	27.746 ug/ml
4)	N-TETRADECANE	8.294	9566644	27.529 ug/ml
5)	N-HEXADECANE	9.896	9501720	27.253 ug/ml
6)	N-OCTADECANE	11.337	9533077	26.958 ug/ml
7)	N-EICOSANE	12.647	9339312	26.555 ug/ml
8)	N-DOCOSANE	13.846	9139260	26.009 ug/ml
10)	N-TETRACOSANE	14.948	8995902	25.414 ug/ml
11)	N-HEXACOSANE	15.968	8696456	24.782 ug/ml
12)	N-OCTACOSANE	16.917	8507317	24.189 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072220\
Data File : FE032443.D
Signal(s) : FID1B.CH
Acq On : 22 Jul 2020 13:58
Operator : DD\AJ
Sample : PB130368BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 23 00:53:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE070720.M
Quant Title :
QLast Update : Wed Jul 08 12:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

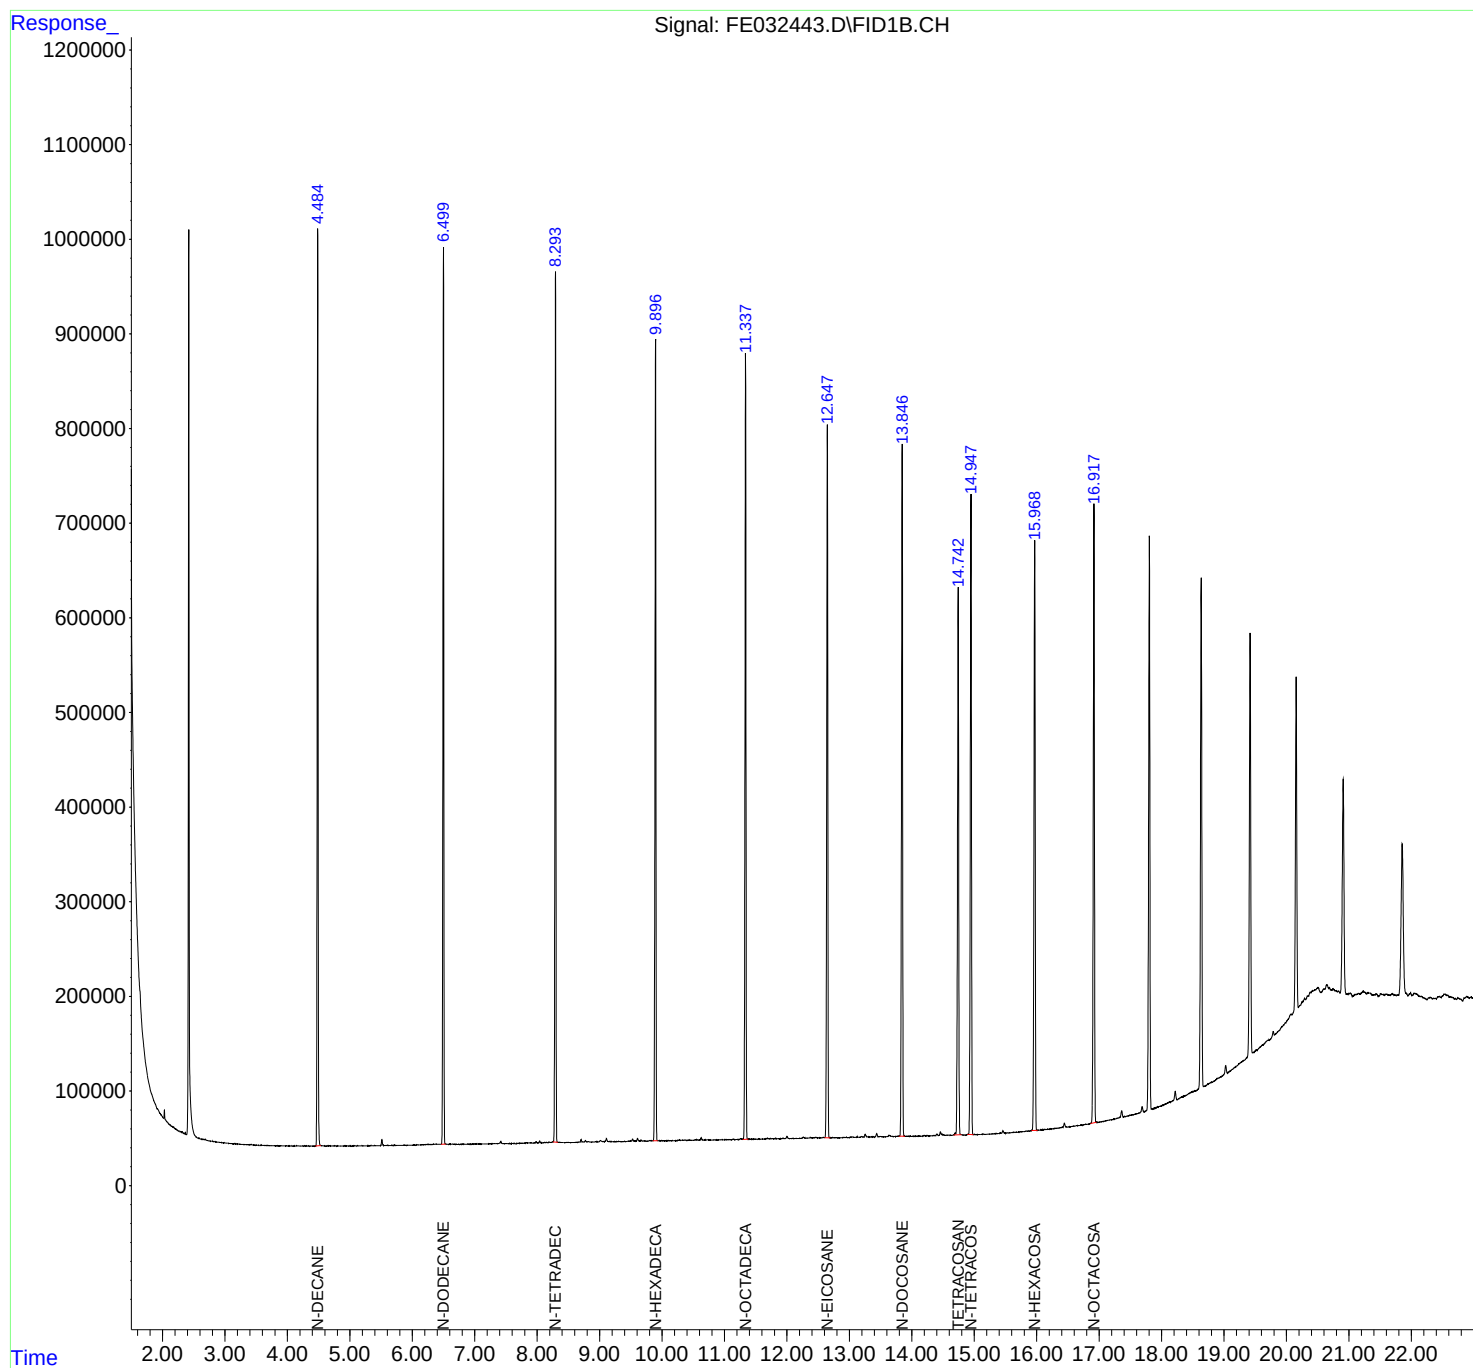

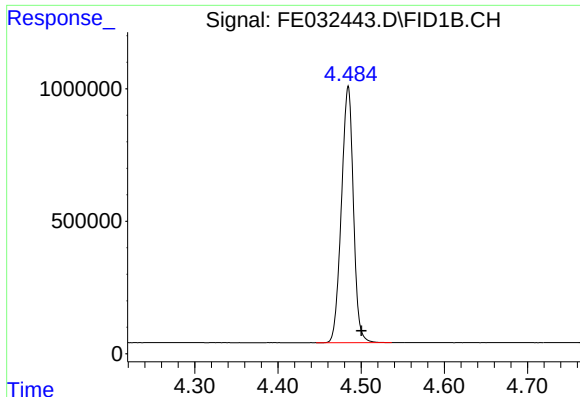


#2 N-DECANE

R.T.: 4.485 min
Delta R.T.: -0.016 min
Response: 9672222
Conc: 27.81 ug/ml

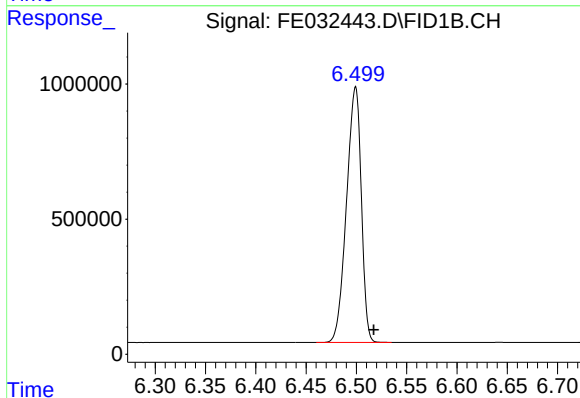


#3 N-DODECANE

R.T.: 6.499 min
Delta R.T.: -0.018 min
Response: 9682784
Conc: 27.75 ug/ml

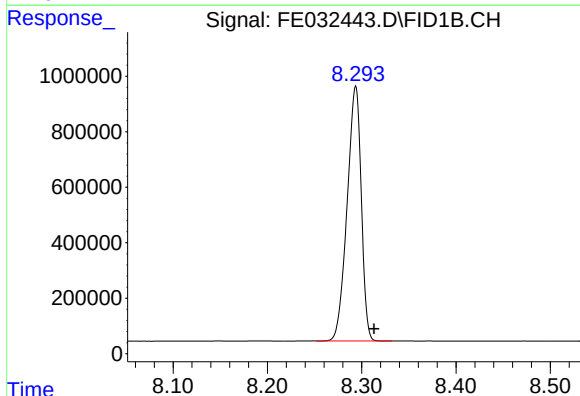


#4 N-TETRADECANE

R.T.: 8.294 min
Delta R.T.: -0.019 min
Response: 9566644
Conc: 27.53 ug/ml

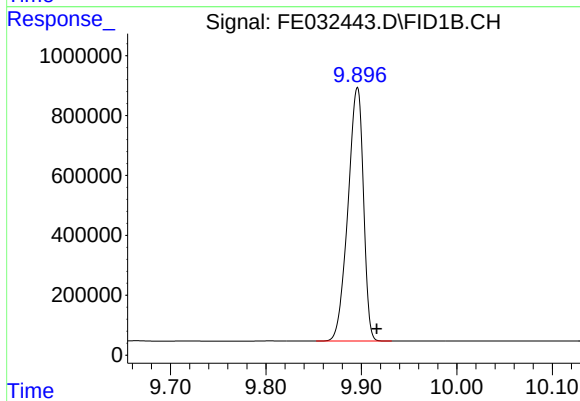


#5 N-HEXADECANE

R.T.: 9.896 min
Delta R.T.: -0.020 min
Response: 9501720
Conc: 27.25 ug/ml

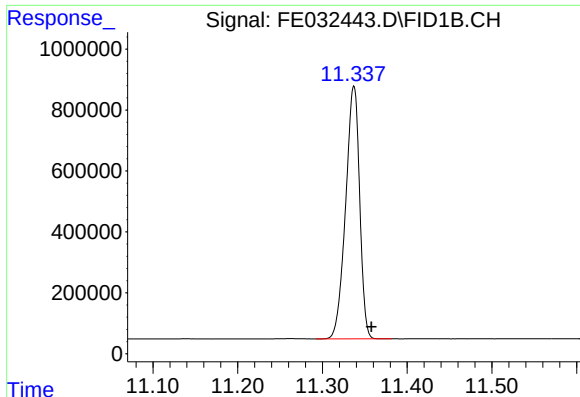


#6 N-OCTADECANE

R.T.: 11.337 min
Delta R.T.: -0.021 min
Response: 9533077
Conc: 26.96 ug/ml

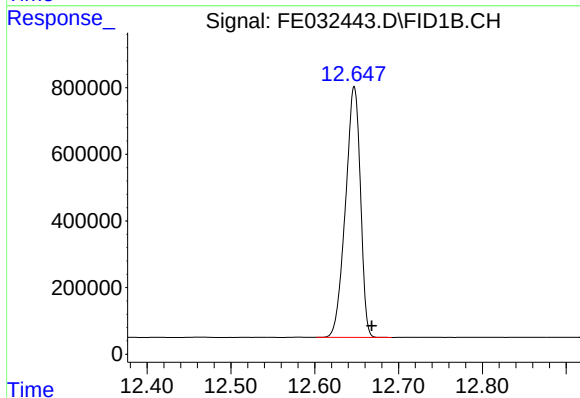


#7 N-EICOSANE

R.T.: 12.647 min
Delta R.T.: -0.021 min
Response: 9339312
Conc: 26.56 ug/ml

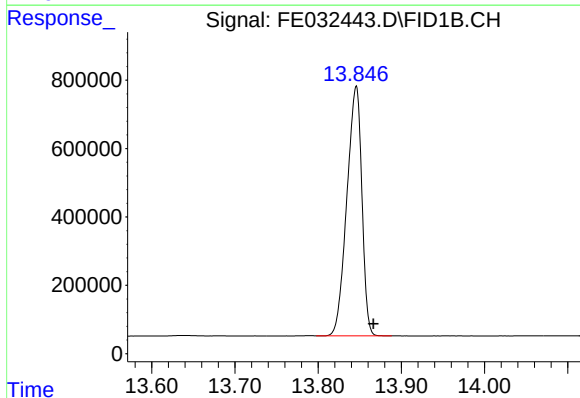


#8 N-DOCOSANE

R.T.: 13.846 min
Delta R.T.: -0.020 min
Response: 9139260
Conc: 26.01 ug/ml

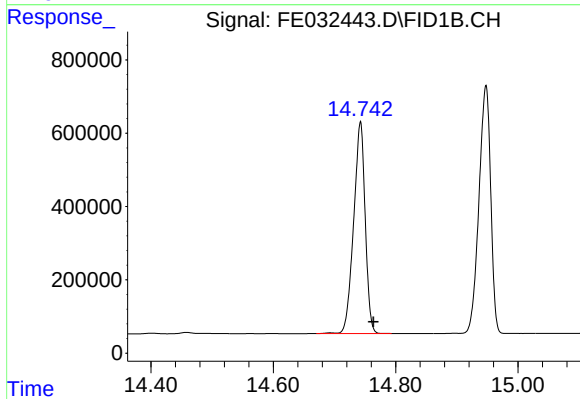


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.743 min
Delta R.T.: -0.021 min
Response: 7557493
Conc: 24.84 ug/ml

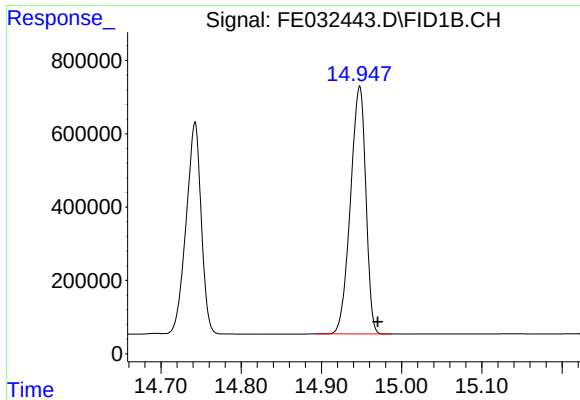


#10 N-TETRACOSANE

R.T.: 14.948 min
Delta R.T.: -0.023 min
Response: 8995902
Conc: 25.41 ug/ml

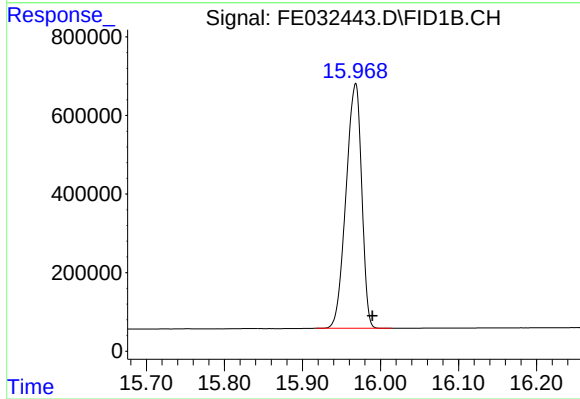

#11 N-HEXACOSANE

R.T.: 15.968 min
Delta R.T.: -0.022 min
Response: 8696456
Conc: 24.78 ug/ml

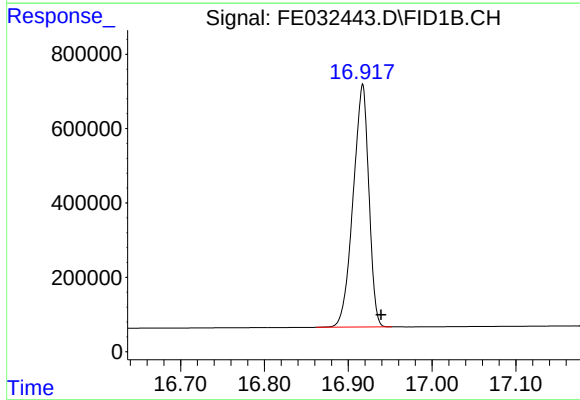

#12 N-OCTACOSANE

R.T.: 16.917 min
Delta R.T.: -0.022 min
Response: 8507317
Conc: 24.19 ug/ml