

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072722\
Data File : FE036727.D
Signal(s) : FID1B.ch
Acq On : 27 Jul 2022 08:33
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 28 01:04:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE072622.M
Quant Title :
QLast Update : Tue Jul 26 14:51:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) N-TETRACOSANE	15.136	48018	0.451 ug/ml
11) N-OCTACOSANE	17.111	46808	0.453 ug/ml
12) N-DOTRIACONTANE	18.832	107053	1.098 ug/ml
14) N-HEXATRIACONTANE	20.357	24874	0.282 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072722\
Data File : FE036727.D
Signal(s) : FID1B.ch
Acq On : 27 Jul 2022 08:33
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 28 01:04:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE072622.M
Quant Title :
QLast Update : Tue Jul 26 14:51:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

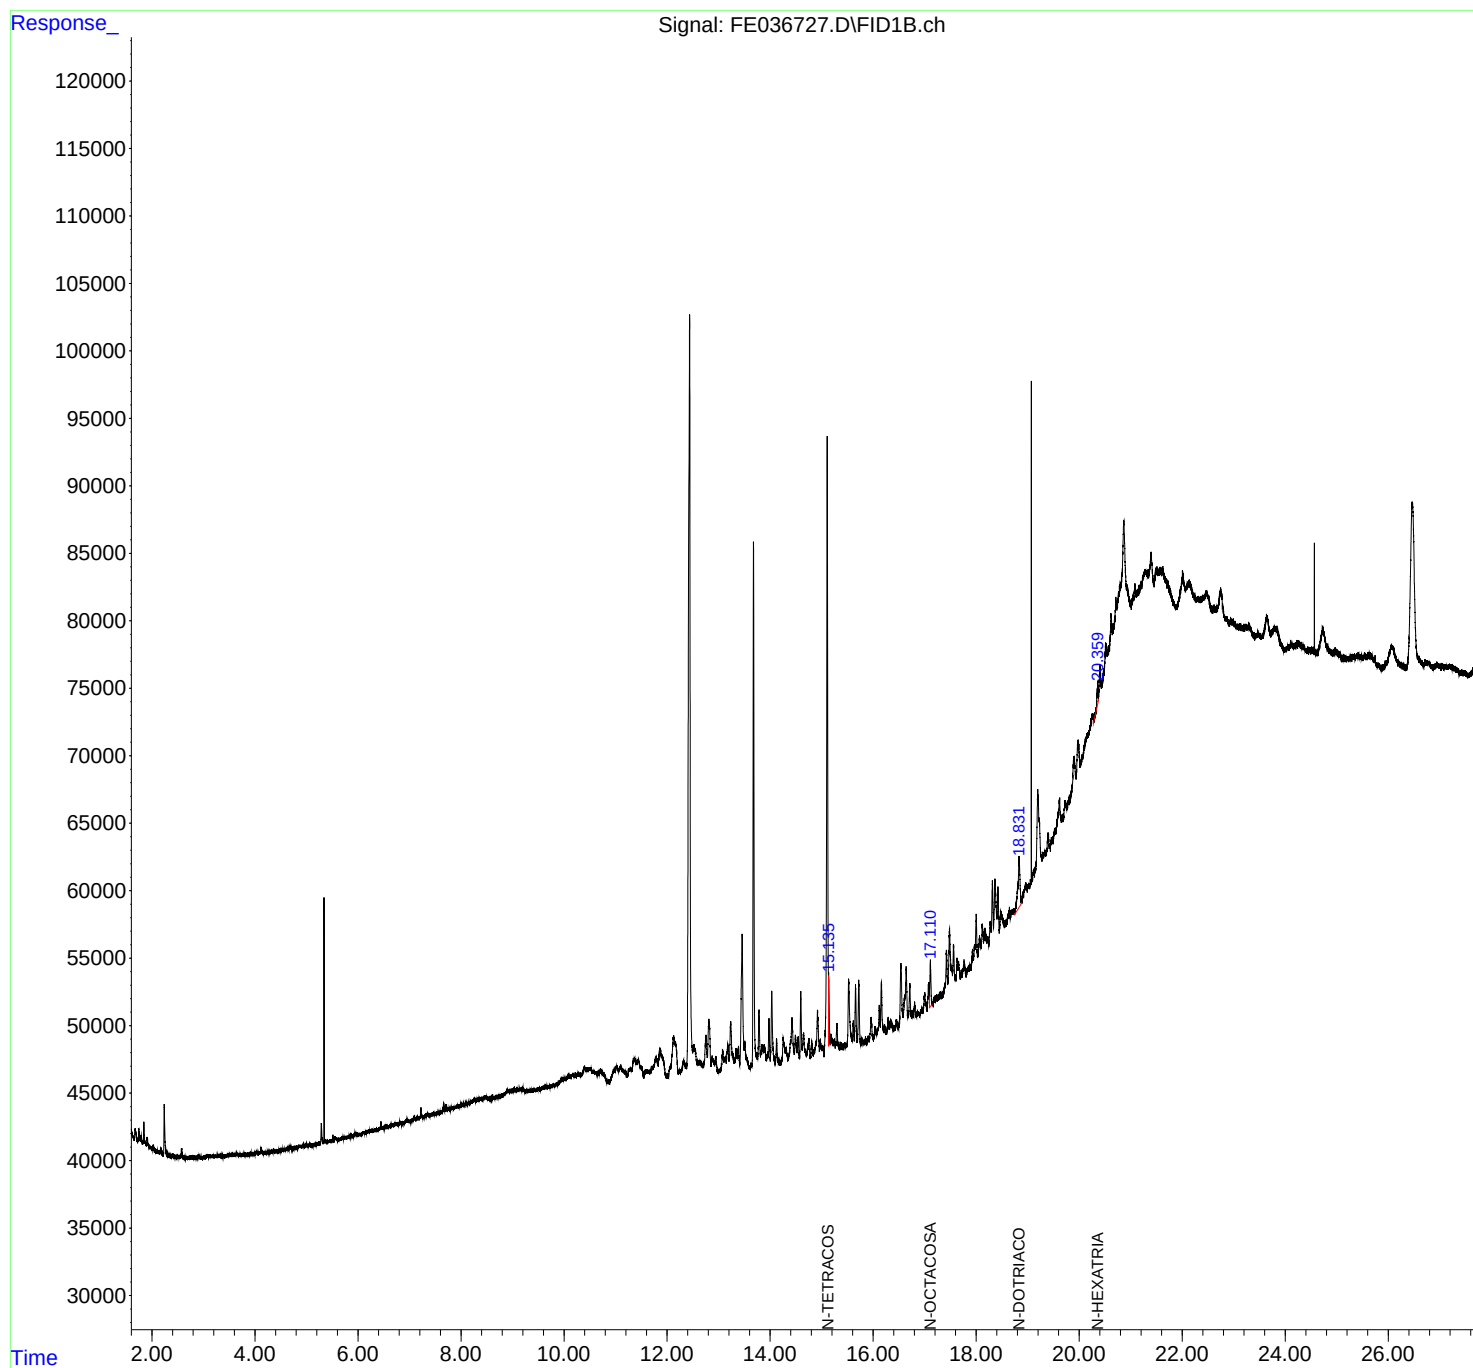


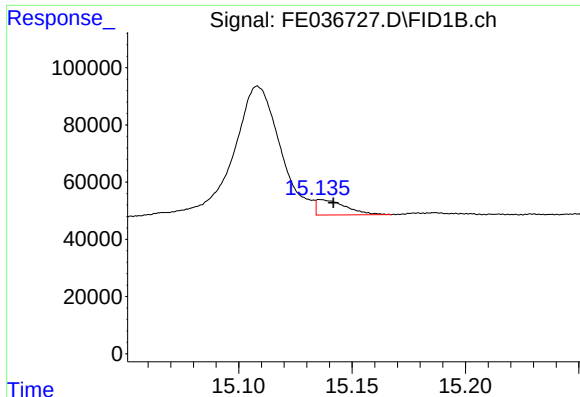

#10 N-TETRACOSANE


R.T.: 15.136 min
Delta R.T.: -0.006 min
Response: 48018
Conc: 0.45 ug/ml

Instrument :
FID_E
ClientSampleId :

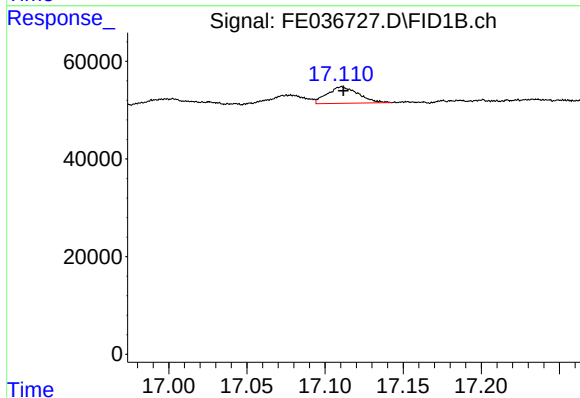


#11 N-OCTACOSANE

R.T.: 17.111 min
Delta R.T.: -0.001 min
Response: 46808
Conc: 0.45 ug/ml

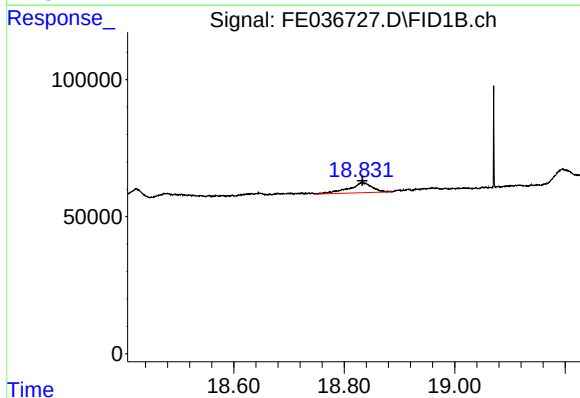


#12 N-DOTRIACONTANE

R.T.: 18.832 min
Delta R.T.: 0.000 min
Response: 107053
Conc: 1.10 ug/ml

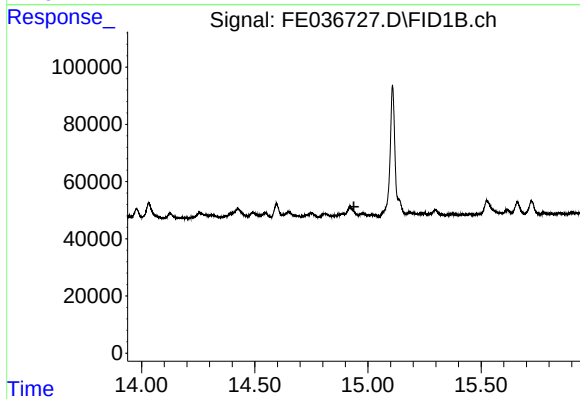

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.938 min
Response: 0
Conc: N.D.

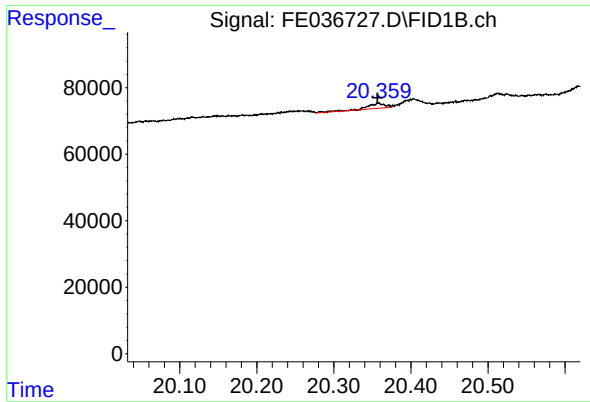

#14 N-HEXATRIACONTANE

R.T.: 20.357 min
Delta R.T.: 0.000 min
Response: 24874
Conc: 0.28 ug/ml

Instrument :

FID_E

ClientSampleId :