

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072722\
Data File : FE036730.D
Signal(s) : FID1B.ch
Acq On : 27 Jul 2022 11:03
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 28 01:05:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE072622.M
Quant Title :
QLast Update : Tue Jul 26 14:51:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
5) N-DODECANE	6.656	2119581	19.579 ug/ml
11) N-OCTACOSANE	17.110	2168953	20.988 ug/ml
12) N-DOTRIACONTANE	18.830	85797	0.880 ug/ml
14) N-HEXATRIACONTANE	20.355	41000	0.466 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072722\
Data File : FE036730.D
Signal(s) : FID1B.ch
Acq On : 27 Jul 2022 11:03
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 28 01:05:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE072622.M
Quant Title :
QLast Update : Tue Jul 26 14:51:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

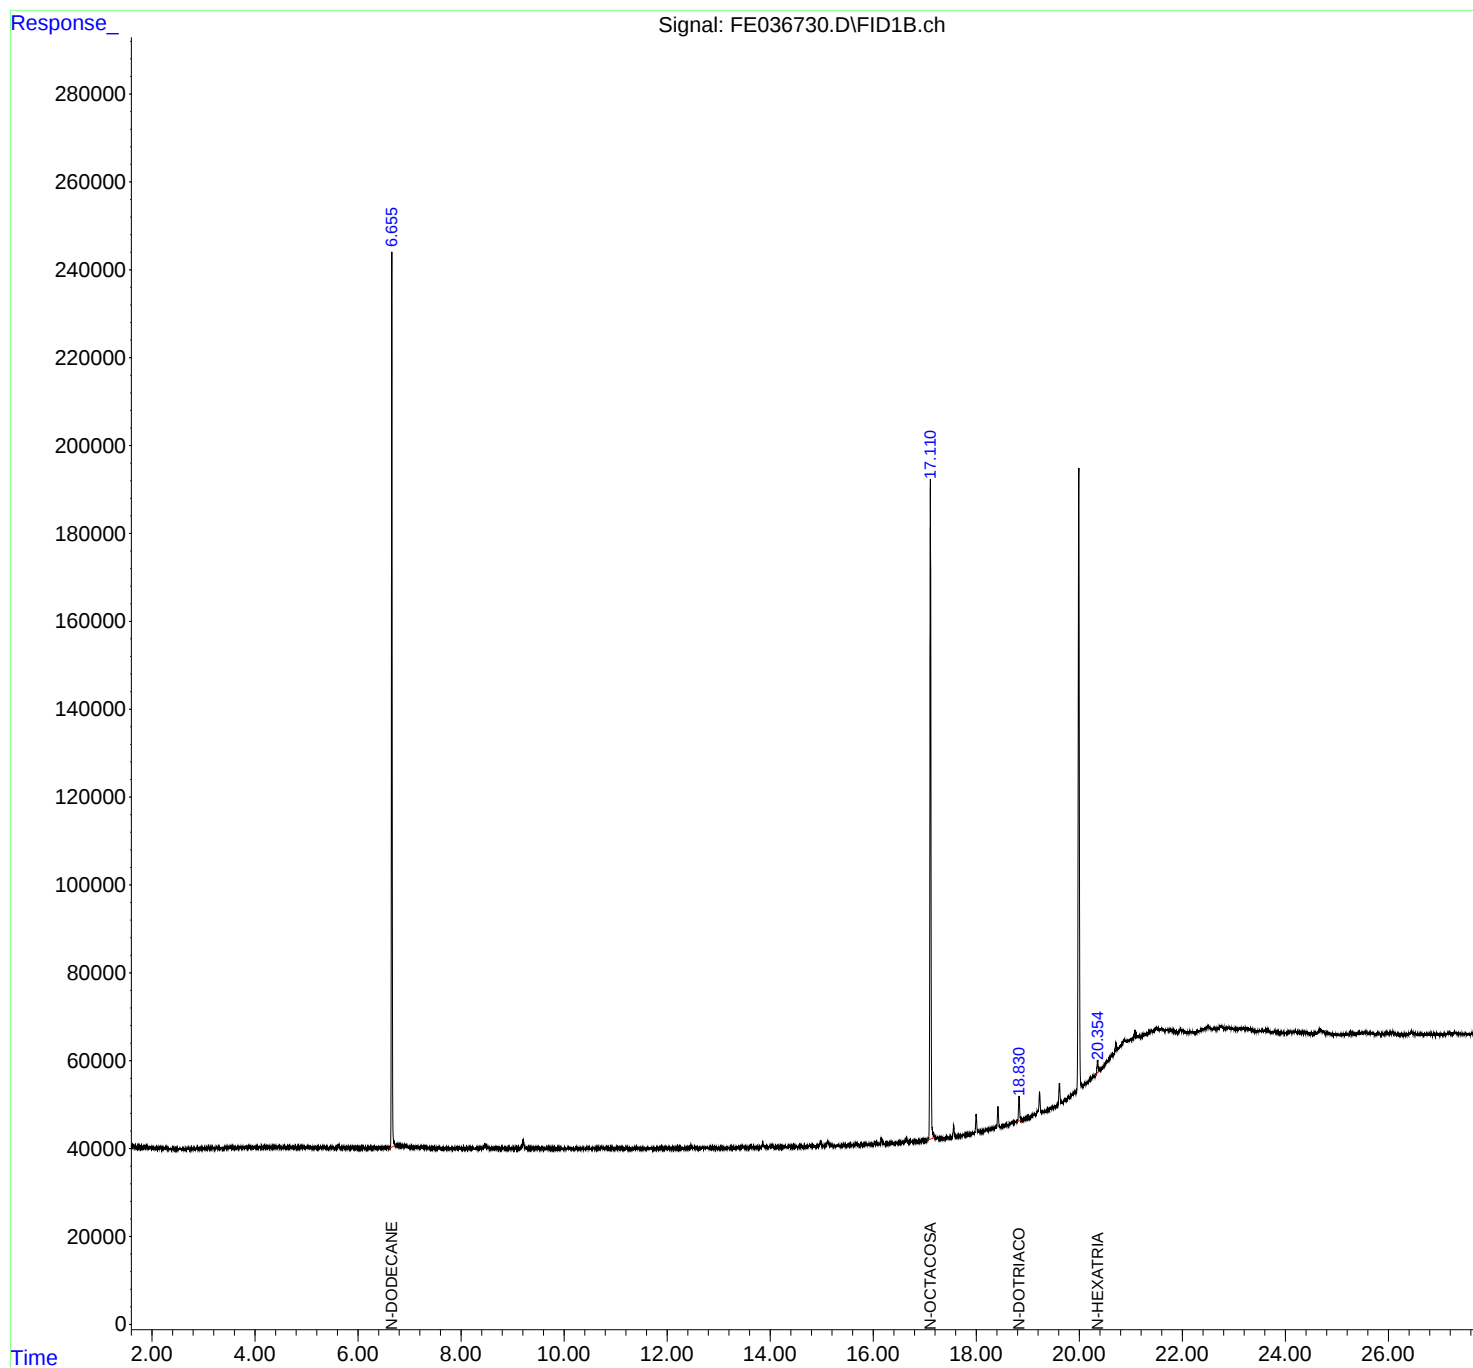


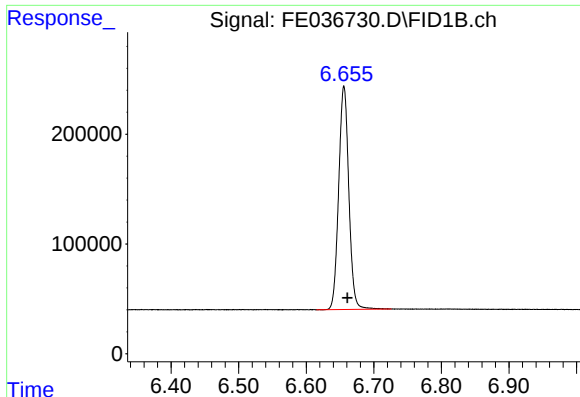

#5 N-DODECANE


R.T.: 6.656 min
Delta R.T.: -0.005 min
Response: 2119581
Conc: 19.58 ug/ml

Instrument :
FID_E
ClientSampleId :

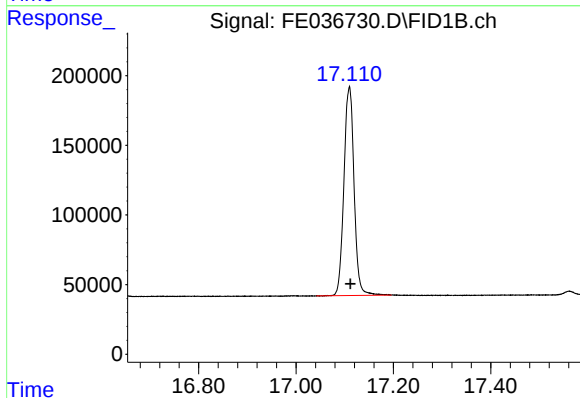


#11 N-OCTACOSANE

R.T.: 17.110 min
Delta R.T.: -0.002 min
Response: 2168953
Conc: 20.99 ug/ml

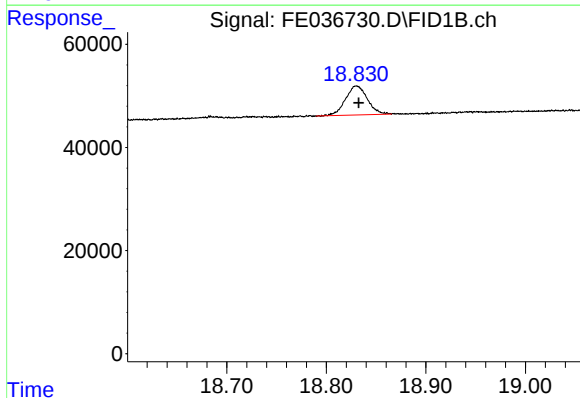


#12 N-DOTRIACONTANE

R.T.: 18.830 min
Delta R.T.: -0.003 min
Response: 85797
Conc: 0.88 ug/ml

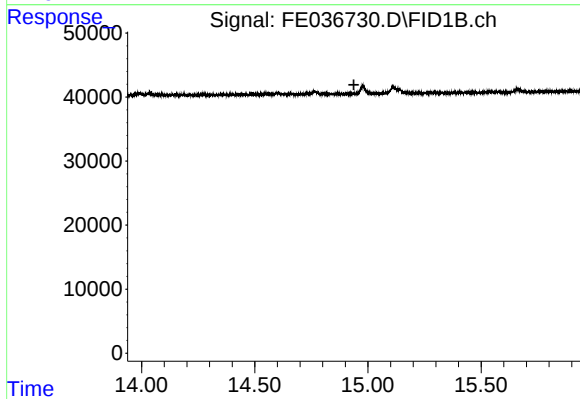

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.938 min
Response: 0
Conc: N.D.

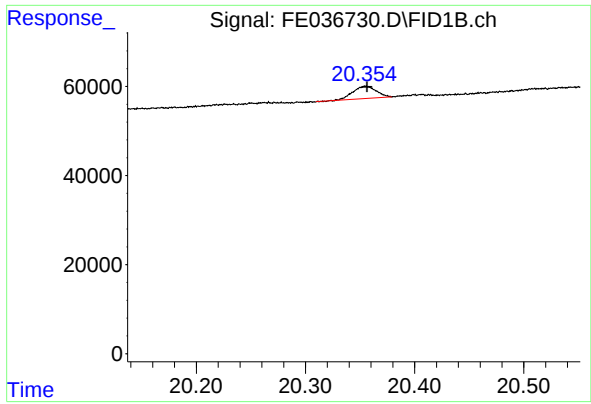

#14 N-HEXATRIACONTANE

R.T.: 20.355 min
Delta R.T.: -0.001 min
Response: 41000
Conc: 0.47 ug/ml

Instrument :

FID_E

ClientSampleId :