

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072722\
 Data File : FE036731.D
 Signal(s) : FID1B.ch
 Acq On : 27 Jul 2022 11:58
 Operator : YP\AJ
 Sample : N3836-02RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 28 01:05:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE072622.M
 Quant Title :
 QLast Update : Tue Jul 26 14:51:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.934	414285	3.173 ug/ml
Target Compounds			
9) N-EICOSANE	12.889	291905	2.709 ug/ml
10) N-TETRACOSANE	15.110	586514	5.504 ug/ml
11) N-OCTACOSANE	17.111	85554	0.828 ug/ml
12) N-DOTRIACONTANE	18.832	123575	1.268 ug/ml
14) N-HEXATRIACONTANE	20.357	21725	0.247 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072722\
Data File : FE036731.D
Signal(s) : FID1B.ch
Acq On : 27 Jul 2022 11:58
Operator : YP\AJ
Sample : N3836-02RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 28 01:05:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE072622.M
Quant Title :
QLast Update : Tue Jul 26 14:51:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

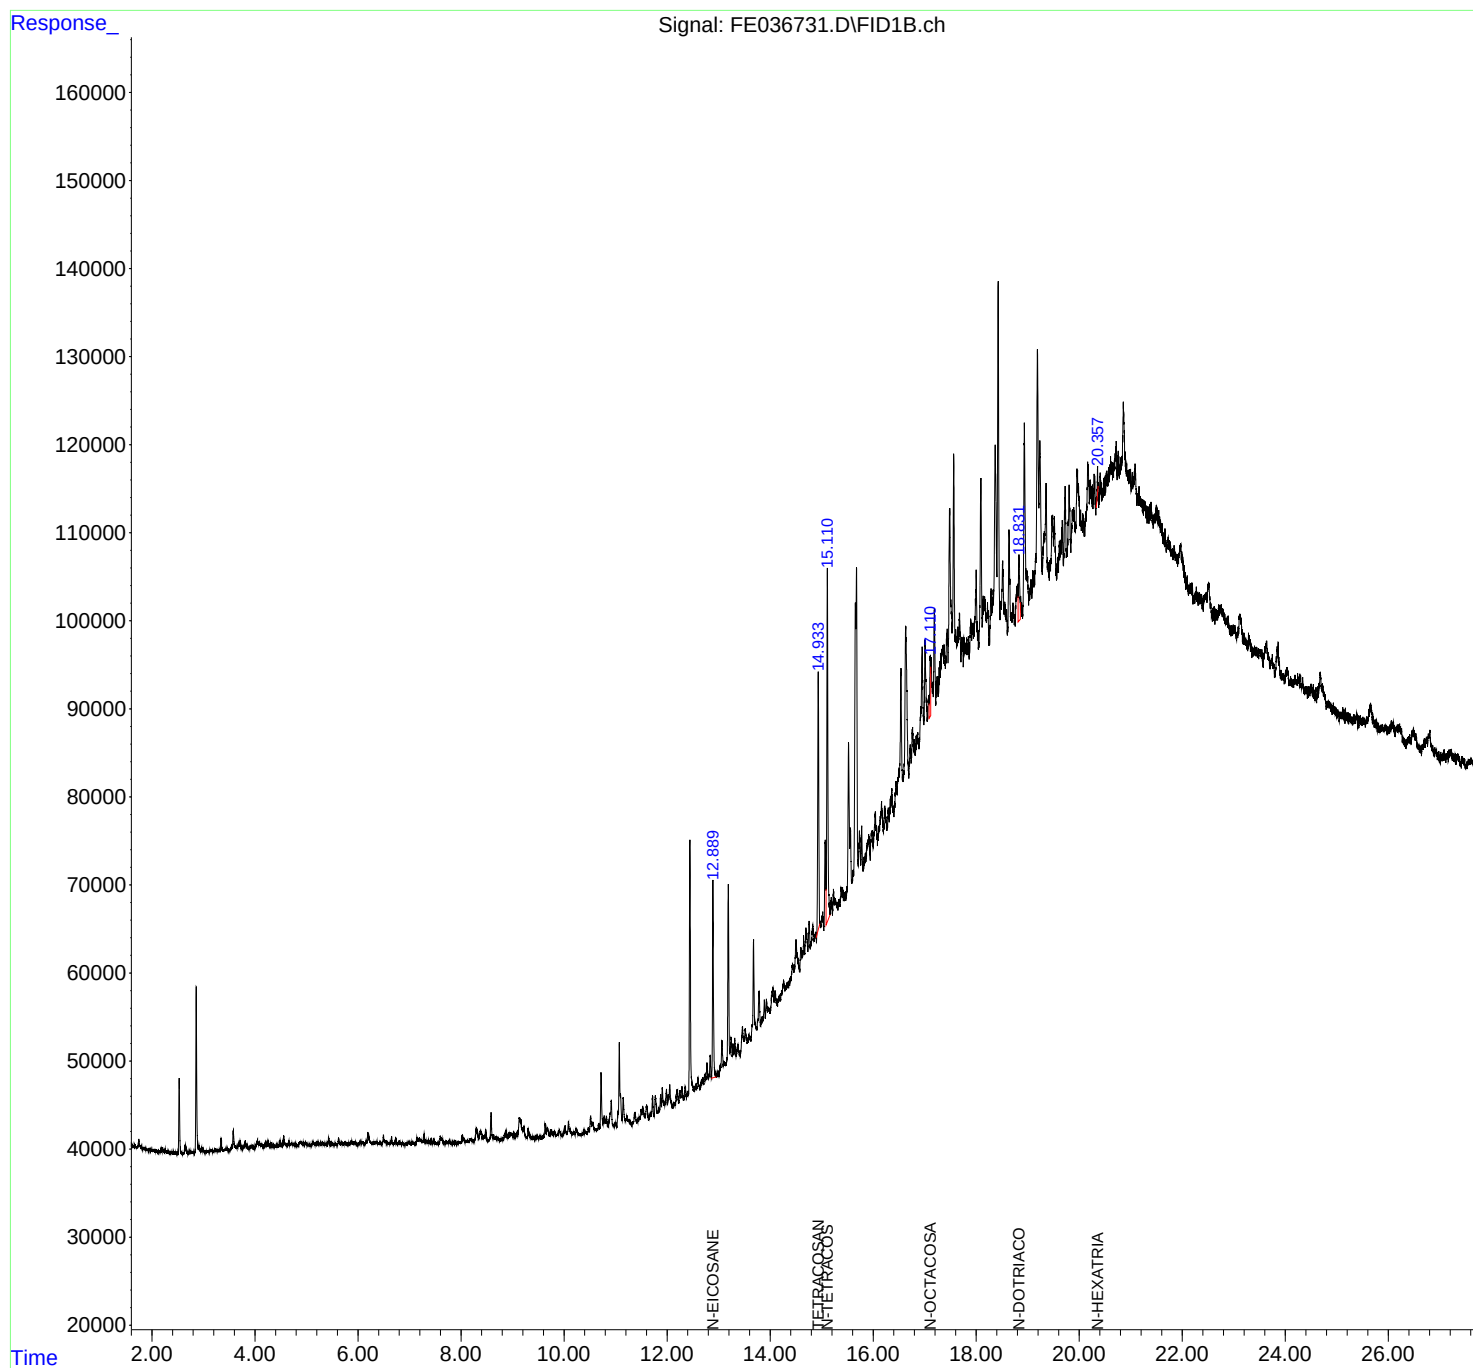


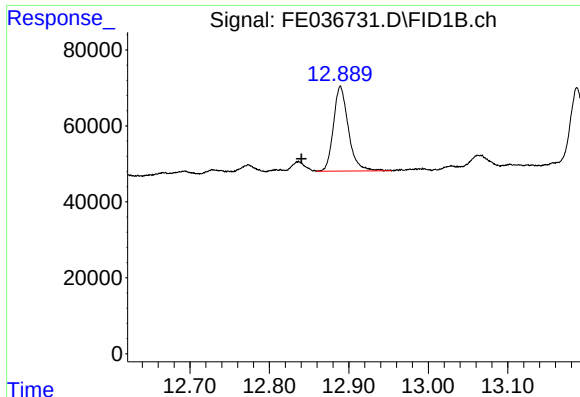

#9 N-EICOSANE


R.T.: 12.889 min
Delta R.T.: 0.049 min
Response: 291905
Conc: 2.71 ug/ml

Instrument :
FID_E
ClientSampleId :

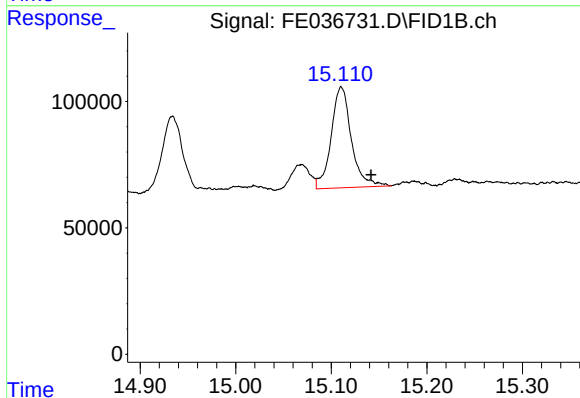


#10 N-TETRACOSANE

R.T.: 15.110 min
Delta R.T.: -0.031 min
Response: 586514
Conc: 5.50 ug/ml

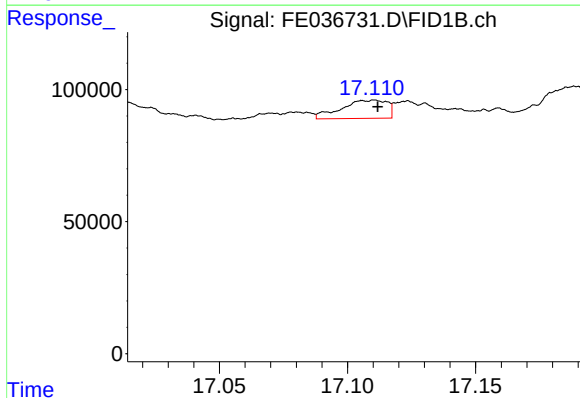


#11 N-OCTACOSANE

R.T.: 17.111 min
Delta R.T.: -0.001 min
Response: 85554
Conc: 0.83 ug/ml

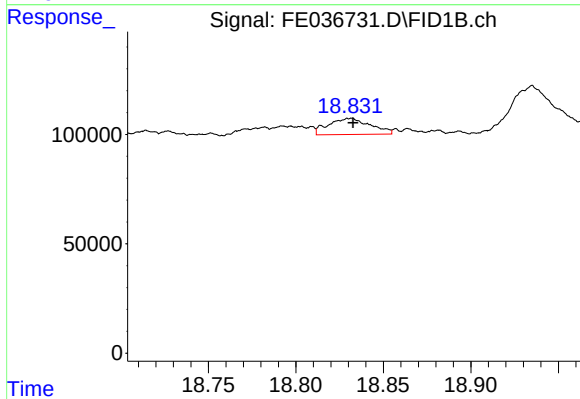

#12 N-DOTRIACONTANE


R.T.: 18.832 min
Delta R.T.: 0.000 min
Response: 123575
Conc: 1.27 ug/ml

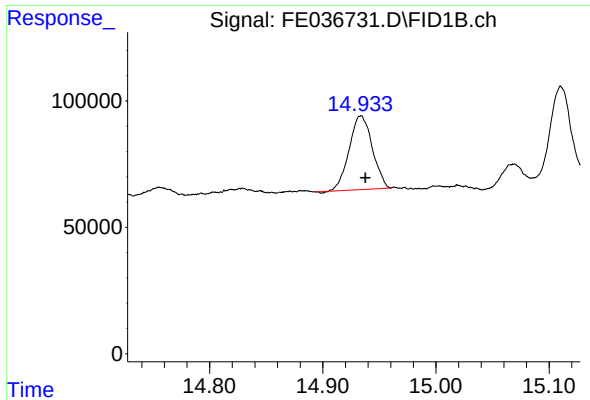

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.934 min
Delta R.T.: -0.004 min
Response: 414285
Conc: 3.17 ug/ml

Instrument :
FID_E
ClientSampleId :

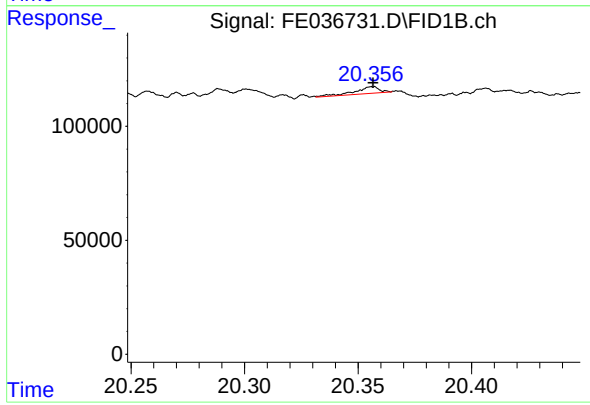

#14 N-HEXATRIACONTANE

R.T.: 20.357 min
Delta R.T.: 0.000 min
Response: 21725
Conc: 0.25 ug/ml