

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072722\
 Data File : FE036733.D
 Signal(s) : FID1B.ch
 Acq On : 27 Jul 2022 13:09
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 28 01:06:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE072622.M
 Quant Title :
 QLast Update : Tue Jul 26 14:51:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.937	2418407	18.525 ug/ml
Target Compounds			
12) N-DOTRIACONTANE	18.830	85212	0.874 ug/ml
14) N-HEXATRIACONTANE	20.360	55526	0.631 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072722\
Data File : FE036733.D
Signal(s) : FID1B.ch
Acq On : 27 Jul 2022 13:09
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 28 01:06:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE072622.M
Quant Title :
QLast Update : Tue Jul 26 14:51:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

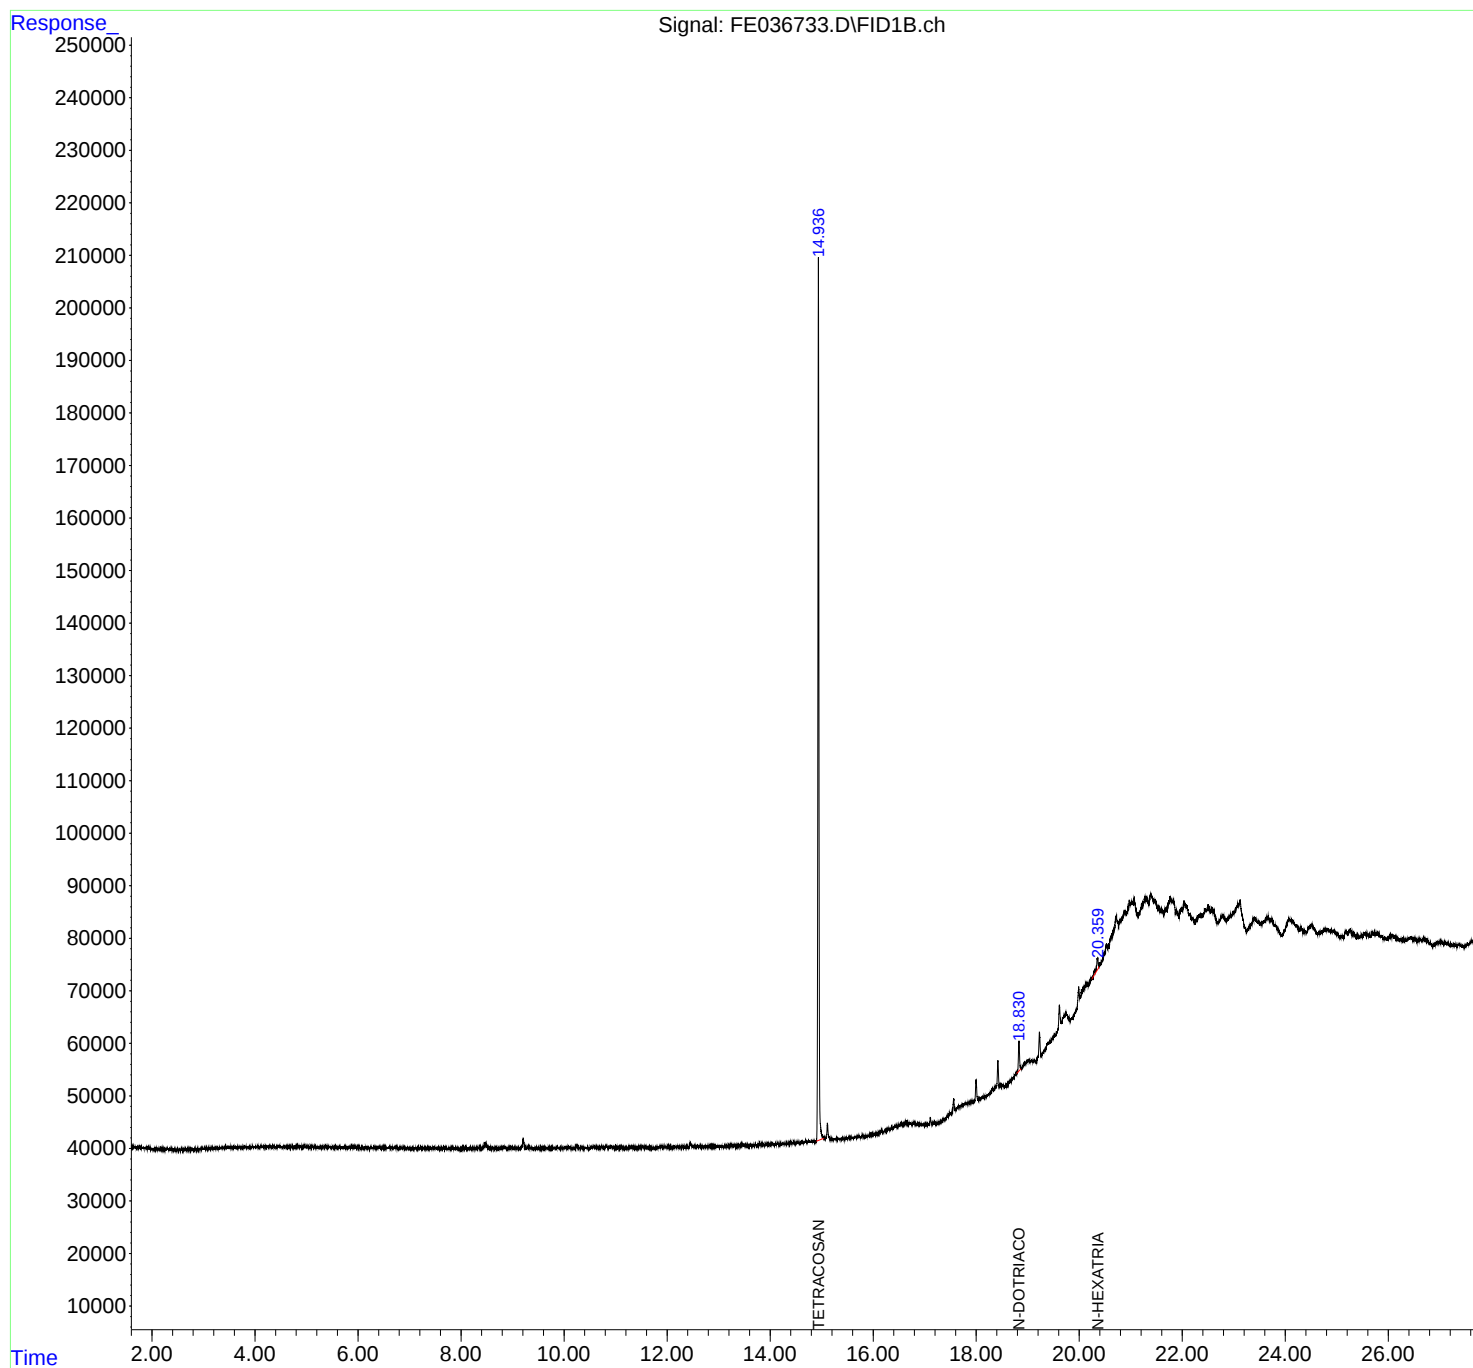


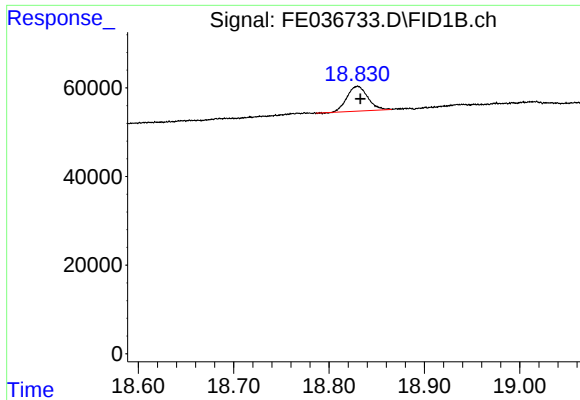

#12 N-DOTRIACONTANE


R.T.: 18.830 min
Delta R.T.: -0.003 min
Response: 85212
Conc: 0.87 ug/ml

Instrument :
FID_E
ClientSampleId :

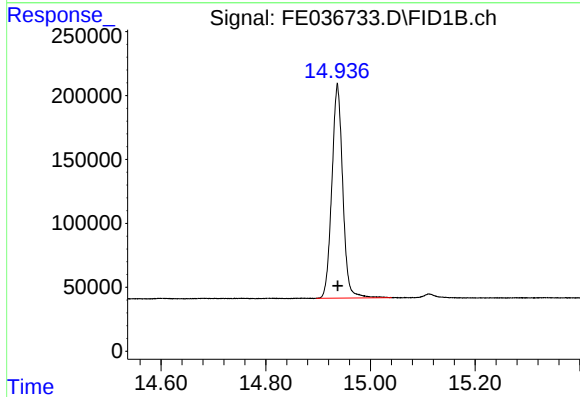

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.937 min
Delta R.T.: 0.000 min
Response: 2418407
Conc: 18.52 ug/ml

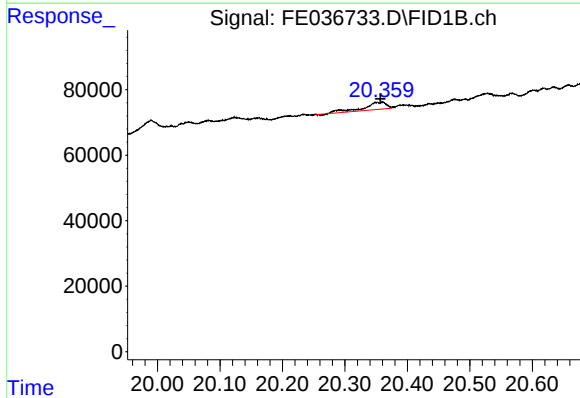

#14 N-HEXATRIACONTANE

R.T.: 20.360 min
Delta R.T.: 0.003 min
Response: 55526
Conc: 0.63 ug/ml