

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072722\
 Data File : FE036731.D
 Signal(s) : FID1B.ch
 Acq On : 27 Jul 2022 11:58
 Operator : YP\AJ
 Sample : N3836-02RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 TP-2RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/28/2022
 Supervised By :Ankita Jodhani 07/28/2022

Integration File: sample.e
 Quant Time: Jul 28 01:05:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE072622.M
 Quant Title :
 QLast Update : Tue Jul 26 14:51:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.933	438395	3.358 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072722\
Data File : FE036731.D
Signal(s) : FID1B.ch
Acq On : 27 Jul 2022 11:58
Operator : YP\AJ
Sample : N3836-02RE
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
TP-2RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/28/2022
Supervised By :Ankita Jodhani 07/28/2022

Integration File: sample.e
Quant Time: Jul 28 01:05:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE072622.M
Quant Title :
QLast Update : Tue Jul 26 14:51:39 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

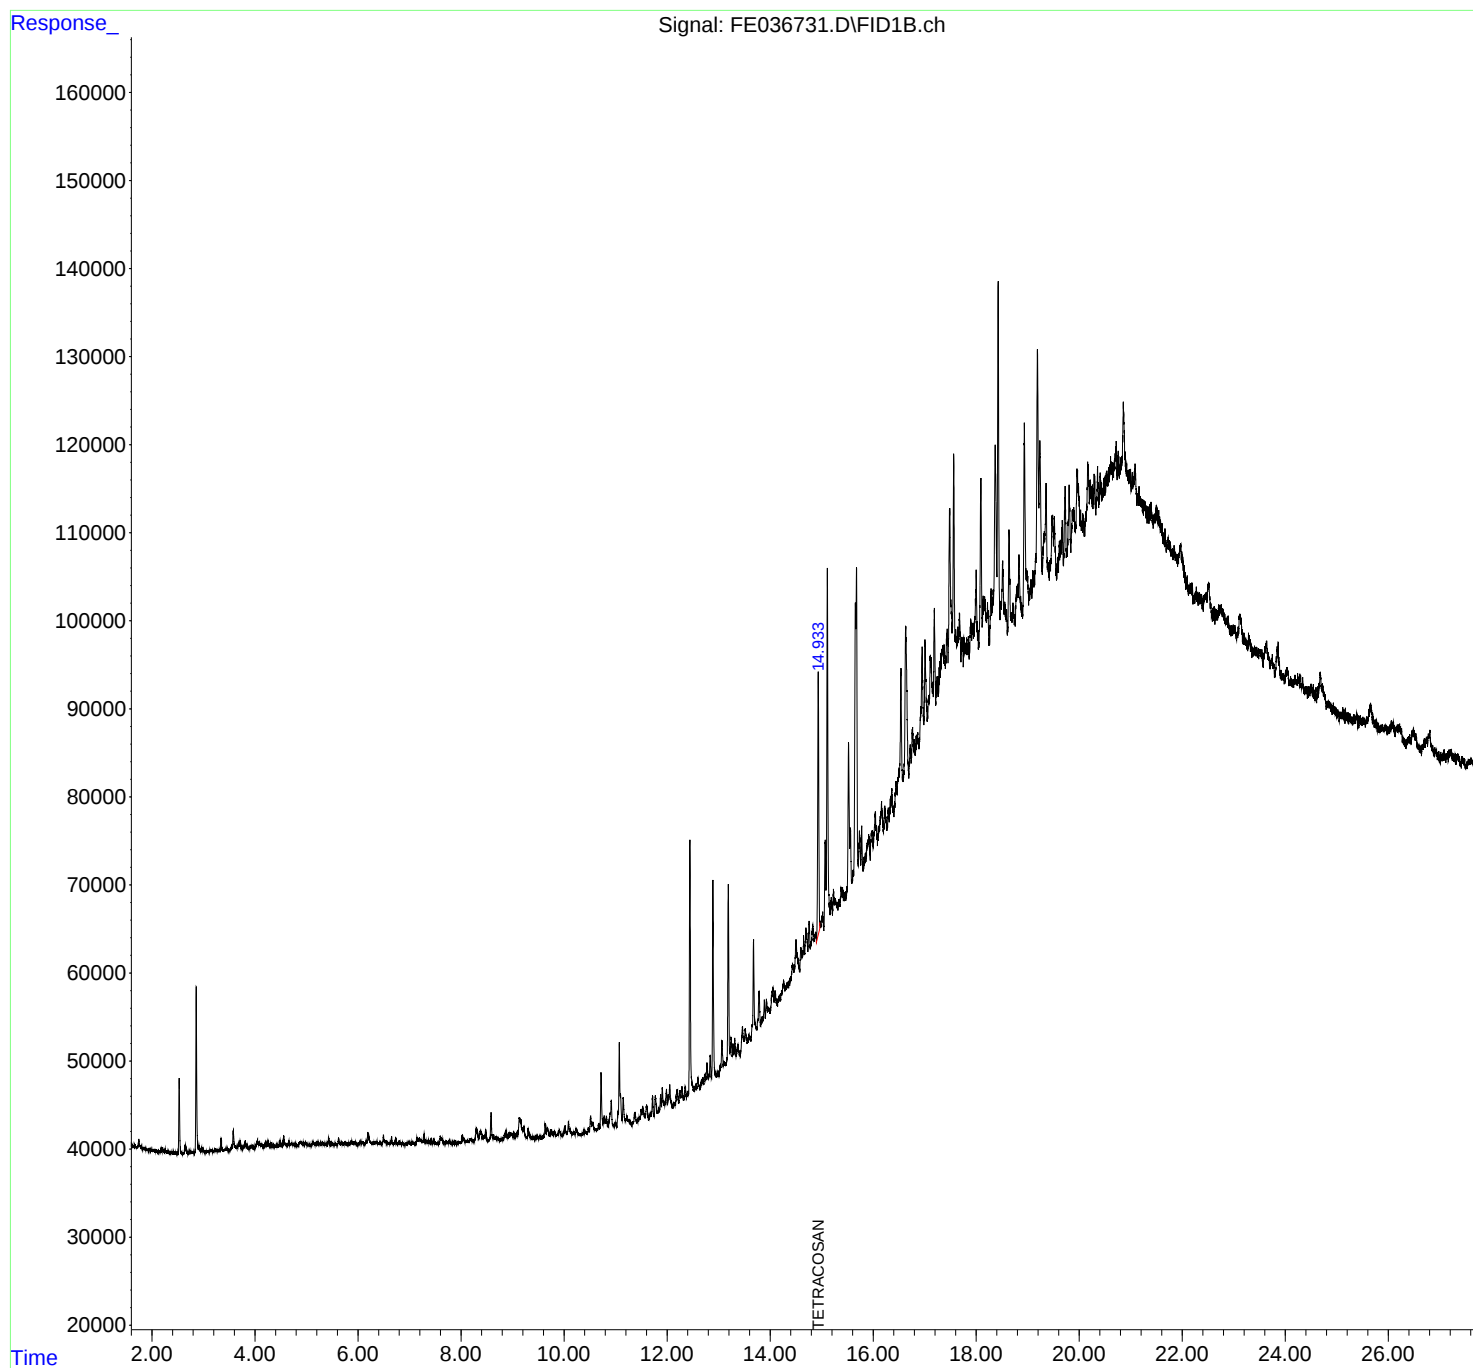

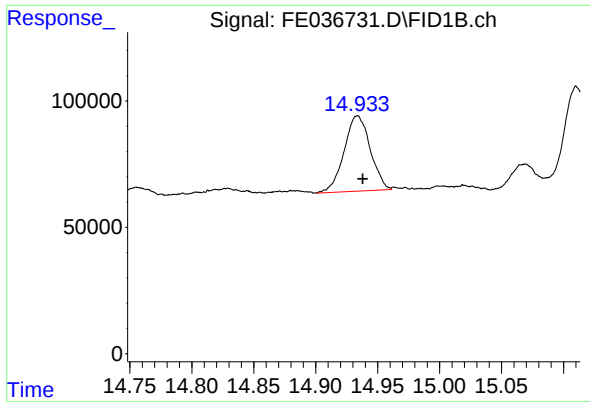

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.933 min
Delta R.T.: -0.004 min
Response: 438395
Conc: 3.36 ug/ml

Instrument :
FID_E
ClientSampleId :
TP-2RE

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/28/2022
Supervised By :Ankita Jodhani 07/28/2022