

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072823AL\
 Data File : FE043623.D
 Signal(s) : FID1B.ch
 Acq On : 29 Jul 2023 05:06
 Operator : YP\AJ
 Sample : 03813-01DL 10X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 PLAUDERVILLE-1DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/31/2023
 Supervised By :Ankita Jodhani 07/31/2023

Integration File: sample.E
 Quant Time: Jul 31 02:11:08 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071323.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 13 03:02:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.883	413125	2.307 ug/ml
Spiked Amount 50.000		Recovery =	4.61%
12) S 1-chlorooctadecane (S...	13.320	304191	2.315 ug/mlm
Spiked Amount 50.000		Recovery =	4.63%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072823AL\
Data File : FE043623.D
Signal(s) : FID1B.ch
Acq On : 29 Jul 2023 05:06
Operator : YP\AJ
Sample : 03813-01DL 10X
Misc :
ALS Vial : 42 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
PLAUDERVILLE-1DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/31/2023
Supervised By :Ankita Jodhani 07/31/2023

Integration File: sample.E
Quant Time: Jul 31 02:11:08 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071323.M
Quant Title : GC Extractables
QLast Update : Thu Jul 13 03:02:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

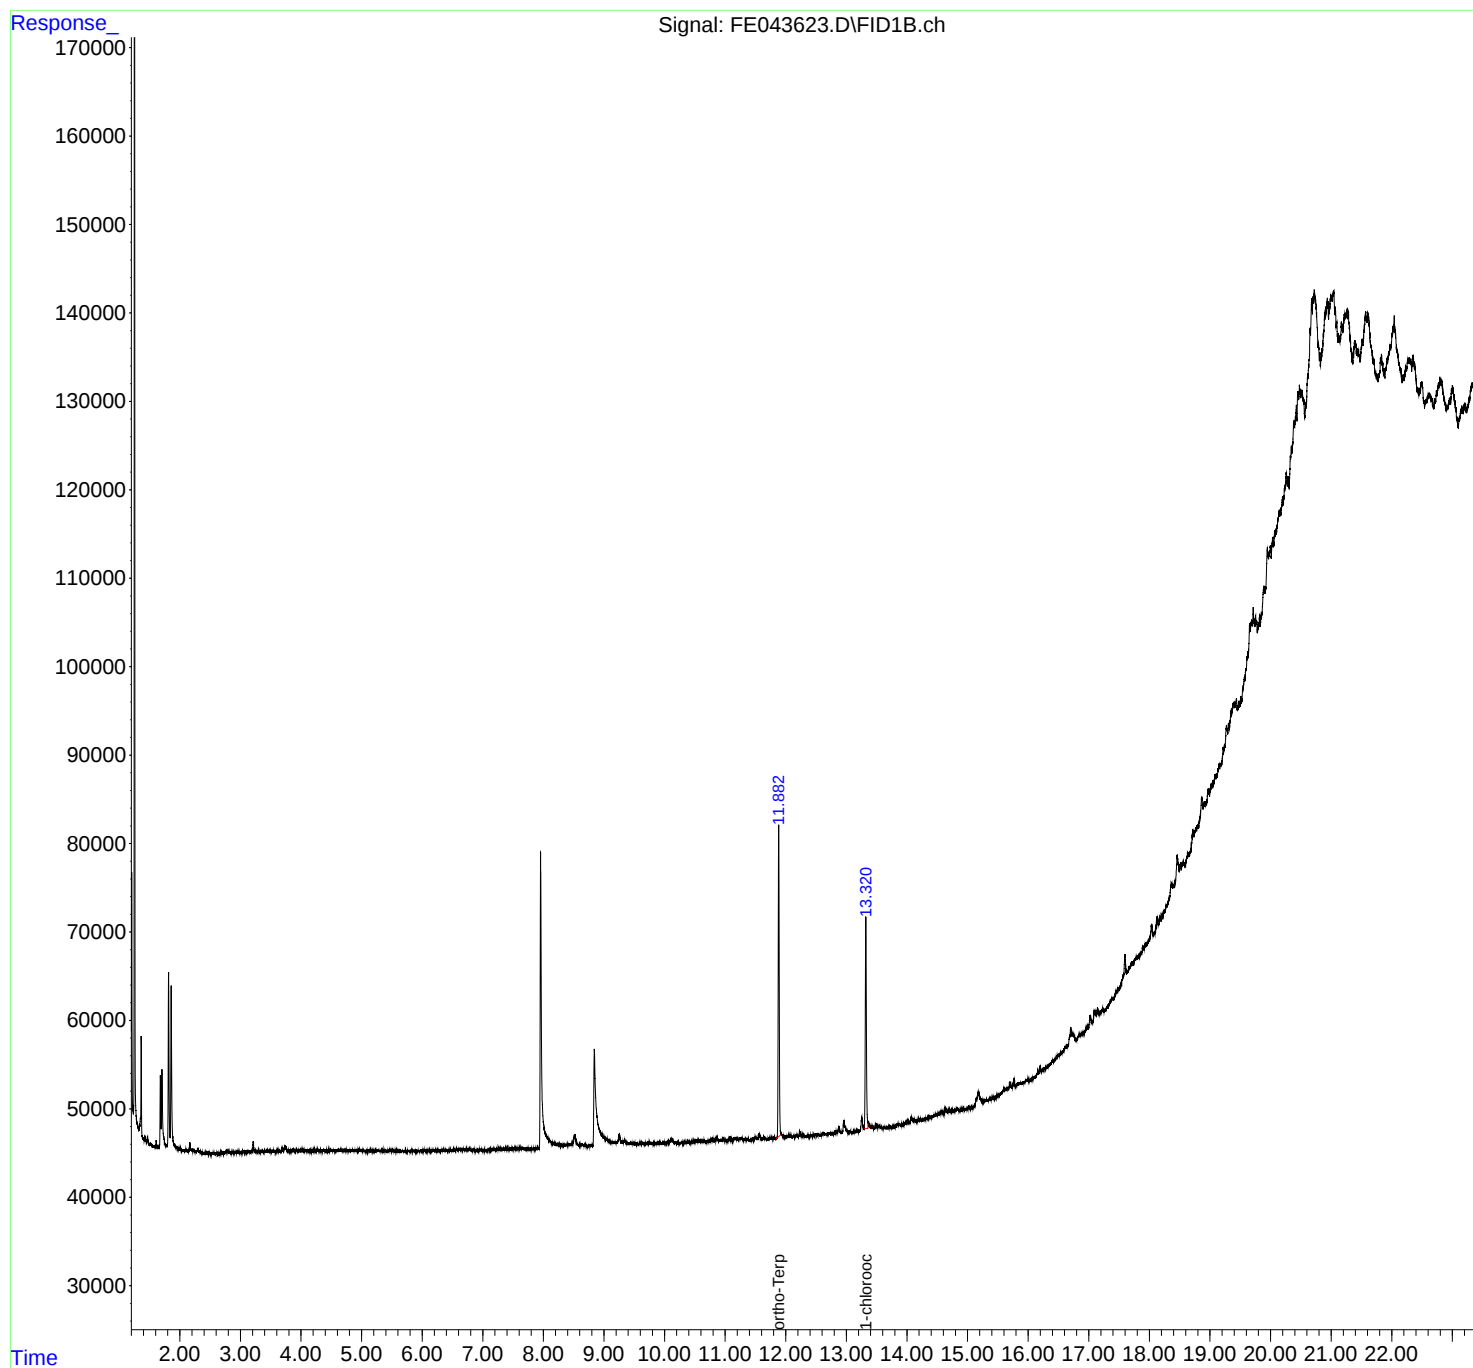

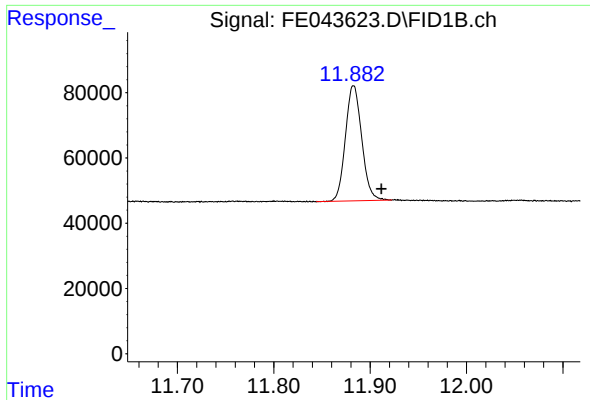

#9 ortho-Terphenyl (SURR)

R.T.: 11.883 min
Delta R.T.: -0.029 min
Response: 413125
Conc: 2.31 ug/ml

Instrument :

FID_E


ClientSampleId :

PLAUDERVILLE-1DL

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/31/2023
Supervised By :Ankita Jodhani 07/31/2023

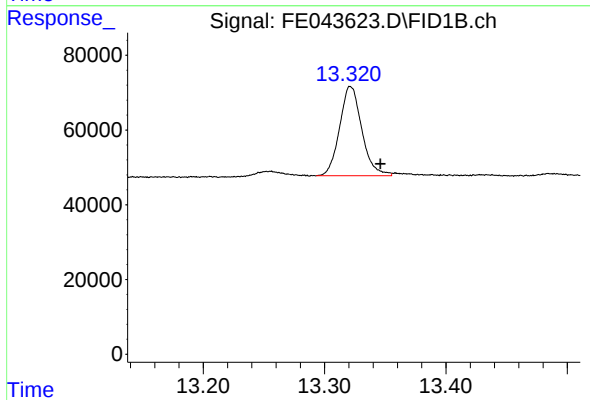

#12 1-chlorooctadecane (SURR)

R.T.: 13.320 min
Delta R.T.: -0.026 min
Response: 304191
Conc: 2.32 ug/ml m