

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072922\
Data File : FE036745.D
Signal(s) : FID1B.ch
Acq On : 28 Jul 2022 09:11
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 28 21:28:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072822.M
Quant Title :
QLast Update : Thu Jul 28 04:33:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.932	2325617	19.048 ug/ml
Target Compounds			
18) N-TETRACONTANE	21.978	541842	4.347 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072922\
Data File : FE036745.D
Signal(s) : FID1B.ch
Acq On : 28 Jul 2022 09:11
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 28 21:28:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072822.M
Quant Title :
QLast Update : Thu Jul 28 04:33:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

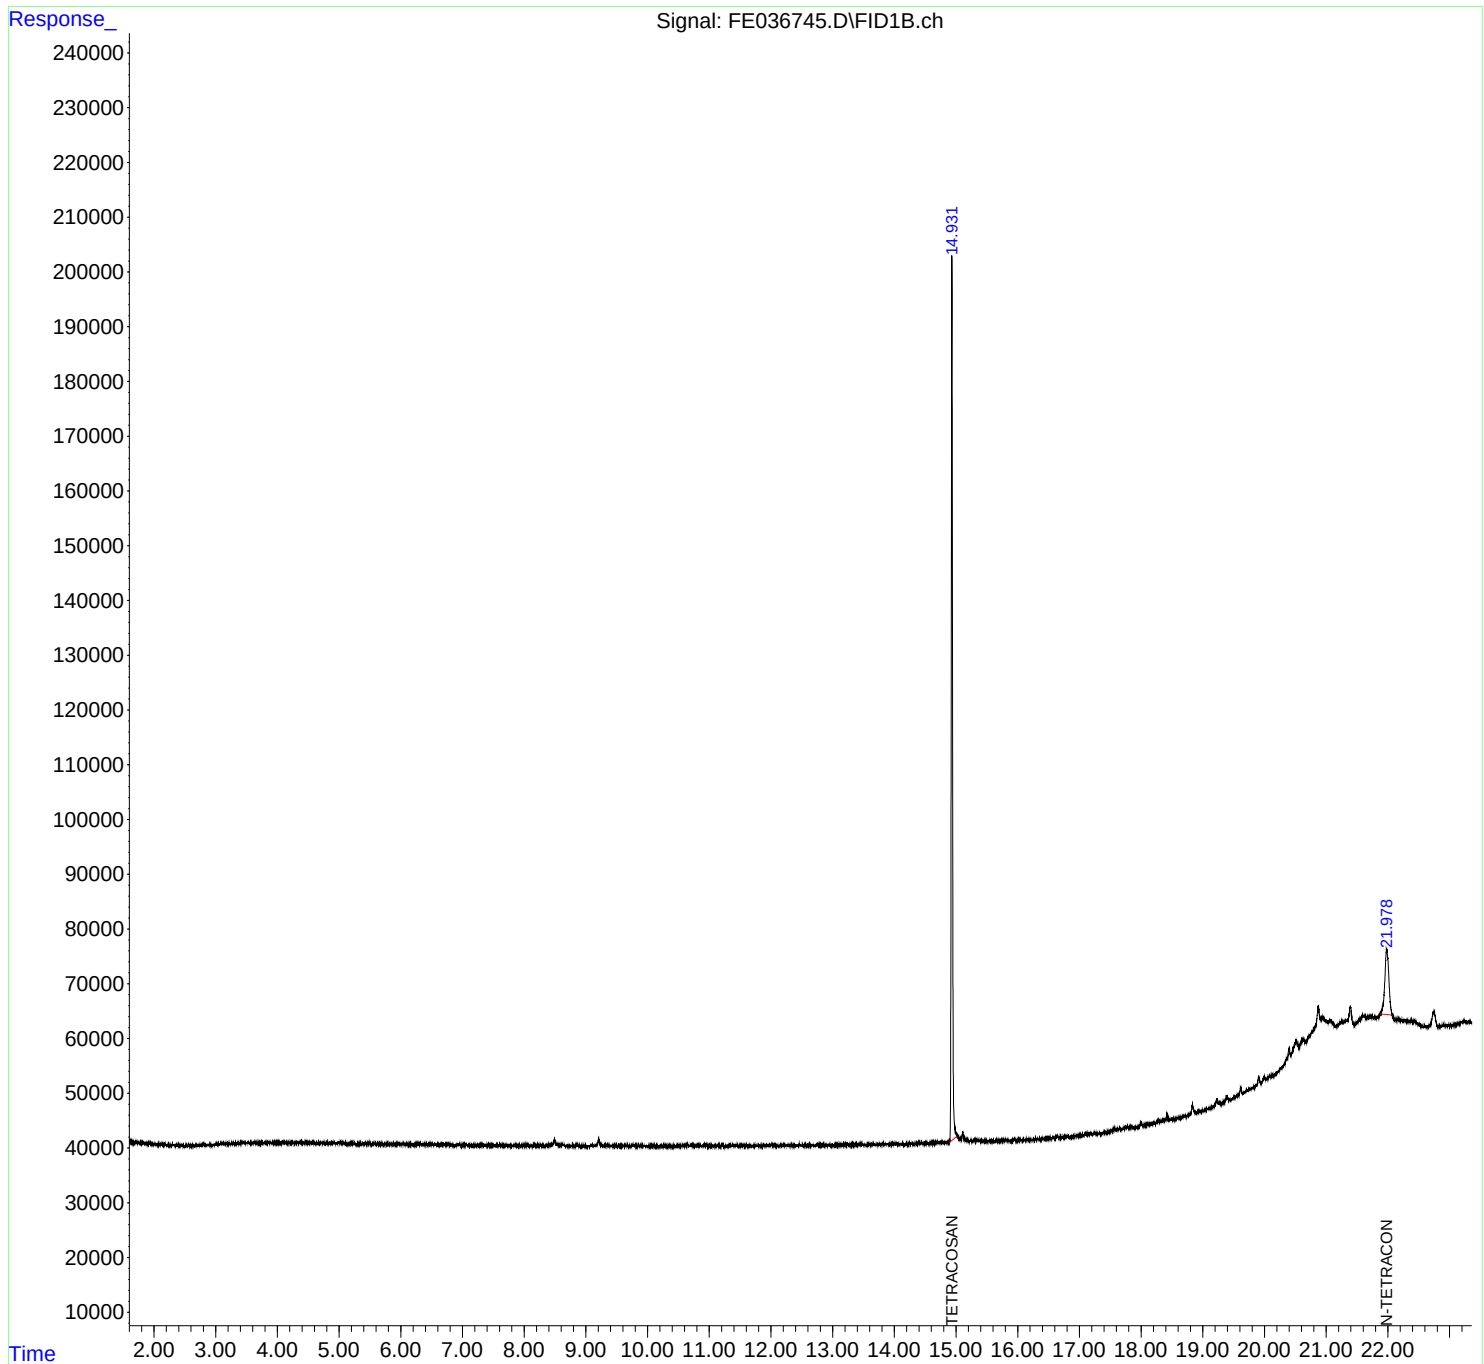


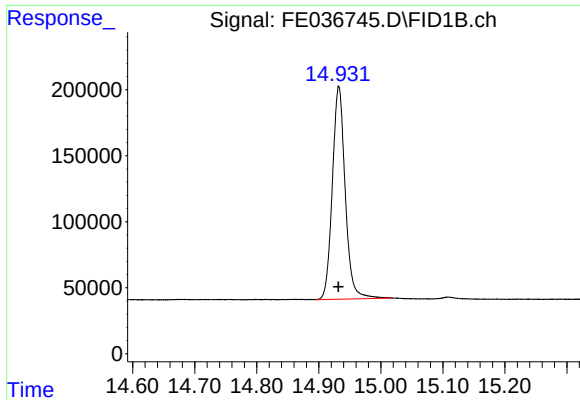

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.932 min
Delta R.T.: 0.000 min
Response: 2325617
Conc: 19.05 ug/ml

Instrument :
FID_E
ClientSampleId :

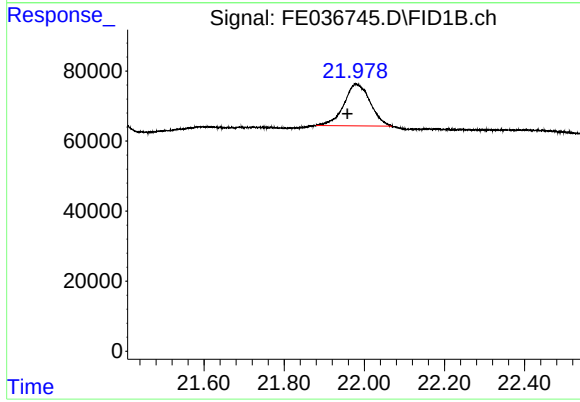

#18 N-TETRACONTANE

R.T.: 21.978 min
Delta R.T.: 0.021 min
Response: 541842
Conc: 4.35 ug/ml