

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072922\
Data File : FE036756.D
Signal(s) : FID1B.ch
Acq On : 28 Jul 2022 16:26
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jul 28 21:30:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072822.M
Quant Title :
QLast Update : Thu Jul 28 04:33:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
3)	N-DODECANE	6.652	1771556	13.039 ug/ml
12)	N-OCTACOSANE	17.107	1892753	14.293 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072922\
Data File : FE036756.D
Signal(s) : FID1B.ch
Acq On : 28 Jul 2022 16:26
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jul 28 21:30:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072822.M
Quant Title :
QLast Update : Thu Jul 28 04:33:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

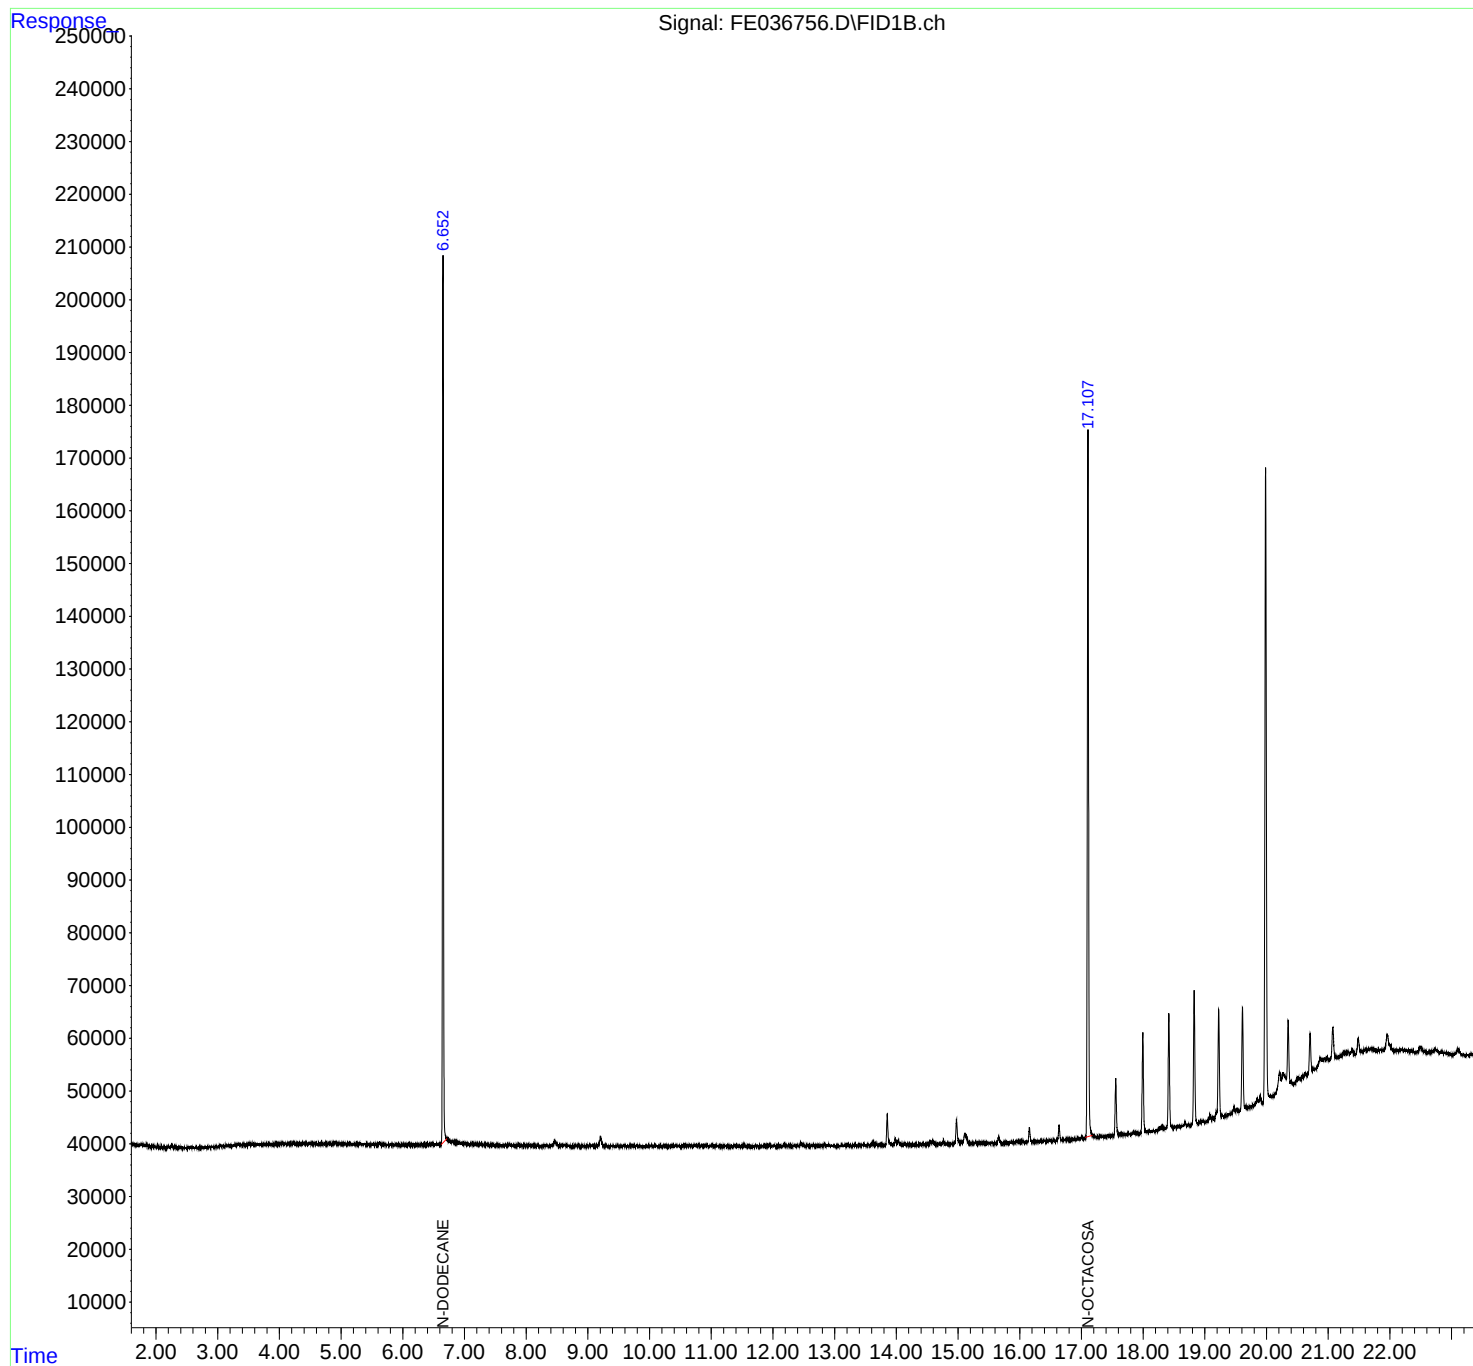


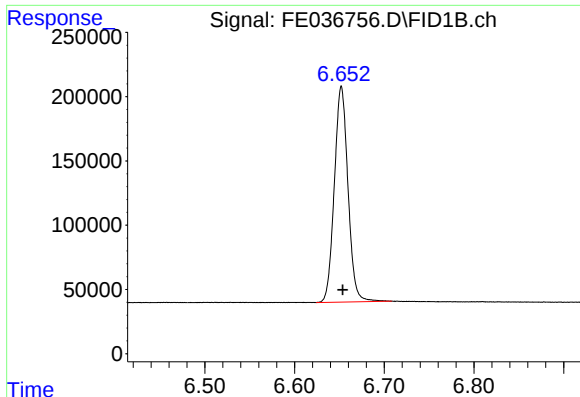

#3 N-DODECANE


R.T.: 6.652 min
Delta R.T.: -0.001 min
Response: 1771556
Conc: 13.04 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

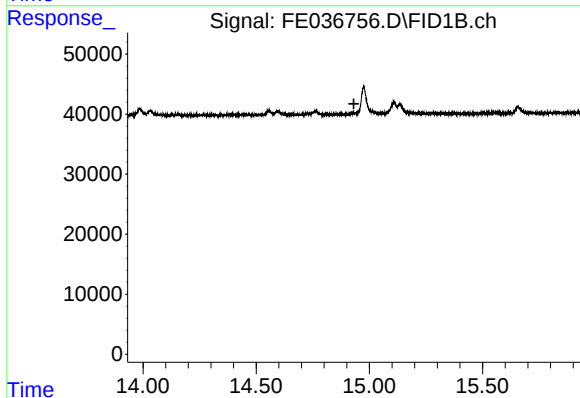

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.932 min
Response: 0
Conc: N.D.

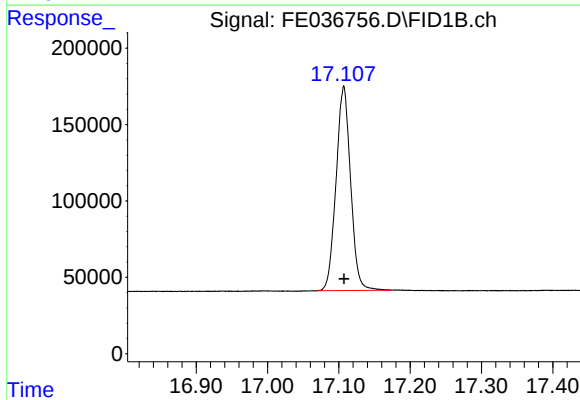

#12 N-OCTACOSANE

R.T.: 17.107 min
Delta R.T.: 0.000 min
Response: 1892753
Conc: 14.29 ug/ml