

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072922\
Data File : FE036759.D
Signal(s) : FID1B.ch
Acq On : 28 Jul 2022 17:59
Operator : YP\AJ
Sample : N3914-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
METRO-DISP

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/29/2022
Supervised By :Ankita Jodhani 07/29/2022

Integration File: autoint1.e
Quant Time: Jul 28 21:32:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072822.M
Quant Title :
QLast Update : Thu Jul 28 04:33:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.914	6061499	49.648 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072922\
Data File : FE036759.D
Signal(s) : FID1B.ch
Acq On : 28 Jul 2022 17:59
Operator : YP\AJ
Sample : N3914-01
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
METRO-DISP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/29/2022
Supervised By :Ankita Jodhani 07/29/2022

Integration File: autoint1.e
Quant Time: Jul 28 21:32:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072822.M
Quant Title :
QLast Update : Thu Jul 28 04:33:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

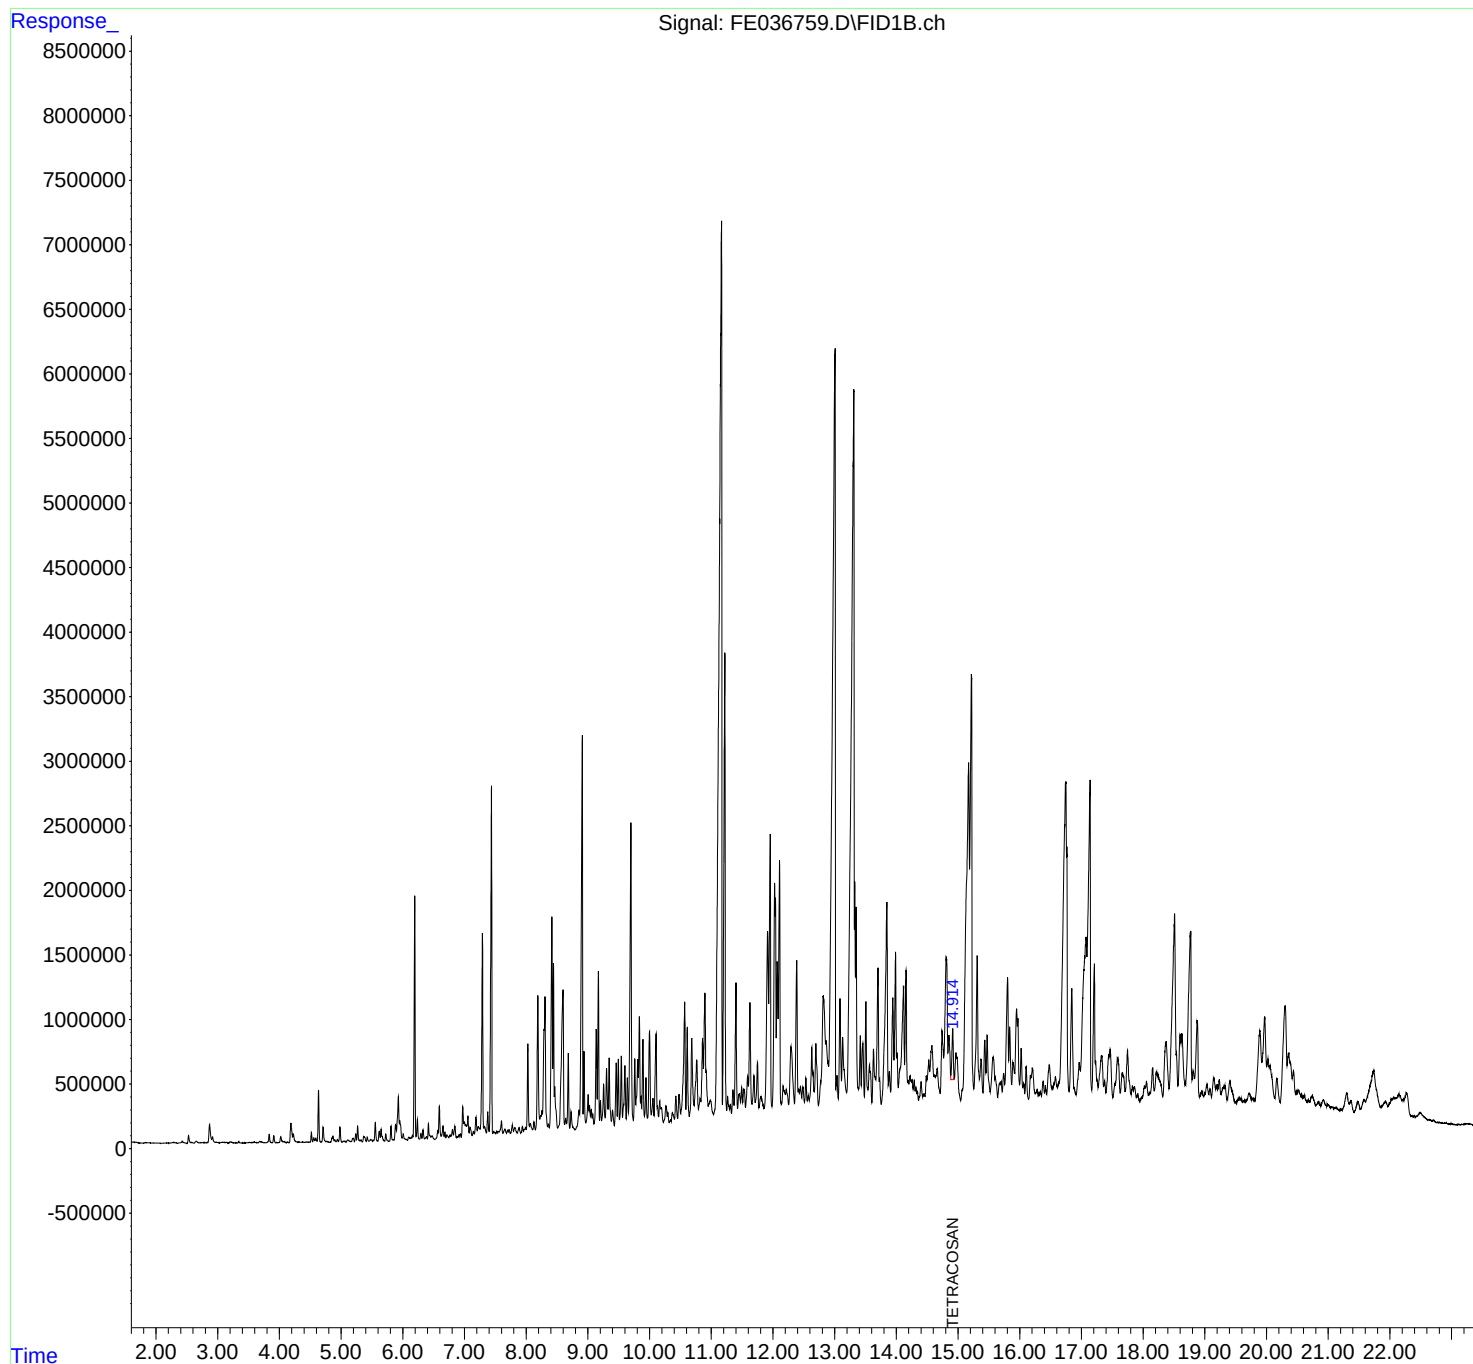

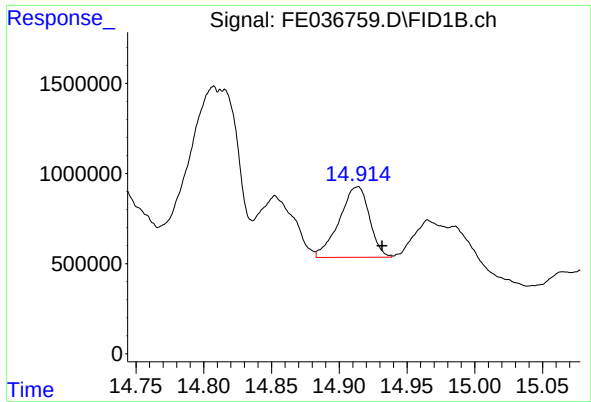

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.914 min
Delta R.T.: -0.018 min
Response: 6061499
Conc: 49.65 ug/ml

Instrument :

FID_E

ClientSampleId :

METRO-DISP

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 07/29/2022
Supervised By :Ankita Jodhani 07/29/2022