

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072922\
Data File : FE036760.D
Signal(s) : FID1B.ch
Acq On : 28 Jul 2022 19:02
Operator : YP\AJ
Sample : N3914-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
METRO-DISP

Integration File: autoint1.e
Quant Time: Jul 28 21:32:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072822.M
Quant Title :
QLast Update : Thu Jul 28 04:33:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.941	1299825	10.646 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE072922\
Data File : FE036760.D
Signal(s) : FID1B.ch
Acq On : 28 Jul 2022 19:02
Operator : YP\AJ
Sample : N3914-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
METRO-DISP

Integration File: autoint1.e
Quant Time: Jul 28 21:32:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072822.M
Quant Title :
QLast Update : Thu Jul 28 04:33:35 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

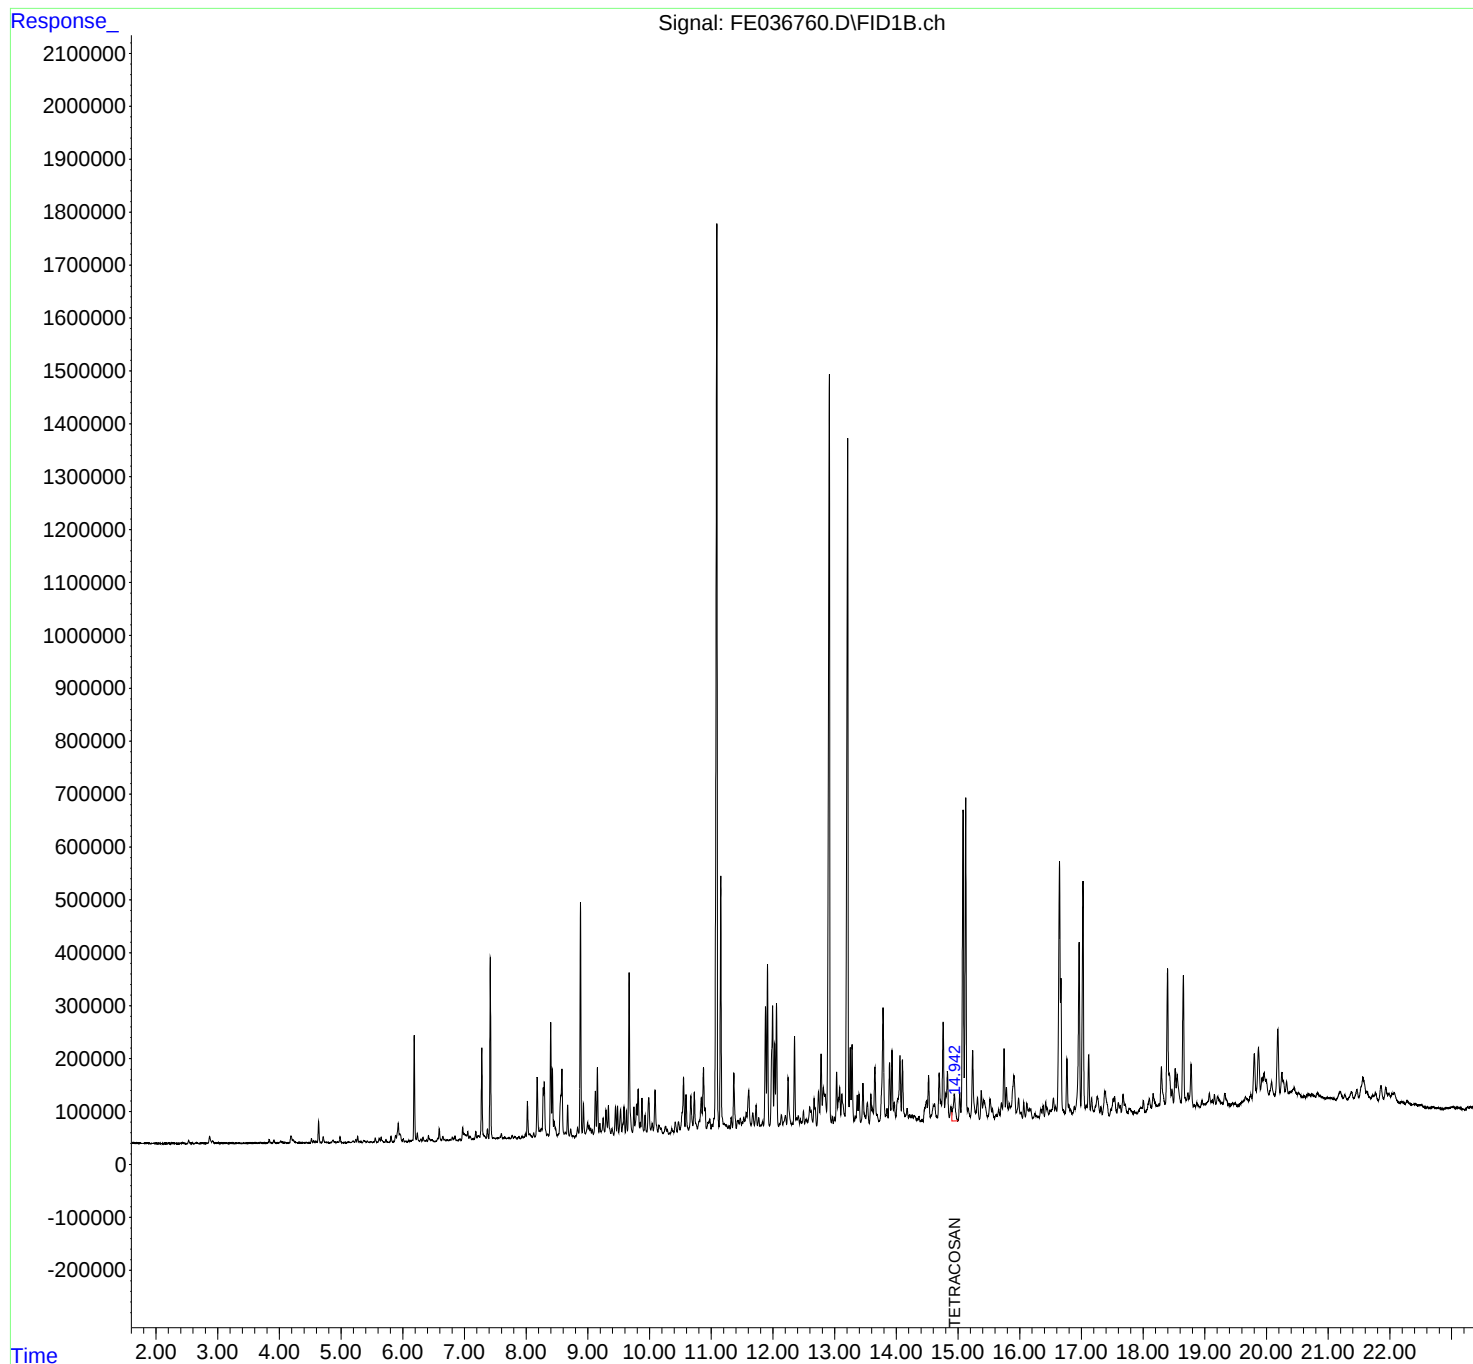

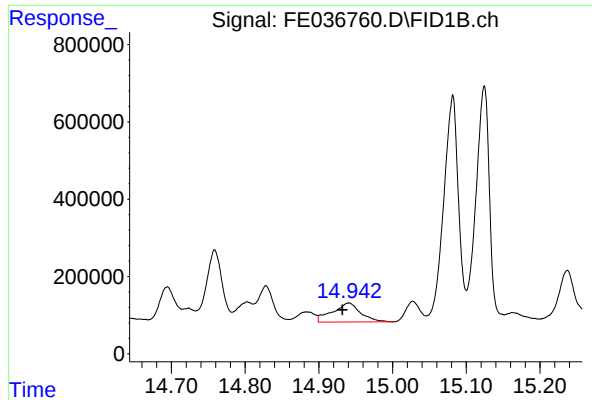

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.941 min
Delta R.T.: 0.009 min
Response: 1299825
Conc: 10.65 ug/ml

Instrument :
FID_E
ClientSampleId :
METRO-DISP