

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE073024AL\  
Data File : FE049318.D  
Signal(s) : FID1B.ch  
Acq On : 30 Jul 2024 19:25  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jul 31 01:22:30 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 071724.M  
Quant Title : GC Extractables  
QLast Update : Wed Jul 17 14:26:40 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound                    |                          | R.T.   | Response | Conc Units  |
|-----------------------------|--------------------------|--------|----------|-------------|
| -----                       |                          |        |          |             |
| System Monitoring Compounds |                          |        |          |             |
| Target Compounds            |                          |        |          |             |
| 18) T                       | n-Dotriacontane (C32)    | 18.885 | 101876   | 0.693 ug/ml |
| 19) T                       | n-Tetratriacontane (C34) | 19.668 | 237591   | 1.627 ug/ml |
| 20) T                       | n-Hexatriacontane (C36)  | 20.405 | 49936    | 0.346 ug/ml |
| 22) T                       | n-Tetracontane (C40)     | 22.092 | 371506   | 2.462 ug/ml |
| -----                       |                          |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE073024AL\  
Data File : FE049318.D  
Signal(s) : FID1B.ch  
Acq On : 30 Jul 2024 19:25  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Jul 31 01:22:30 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 071724.M  
Quant Title : GC Extractables  
QLast Update : Wed Jul 17 14:26:40 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

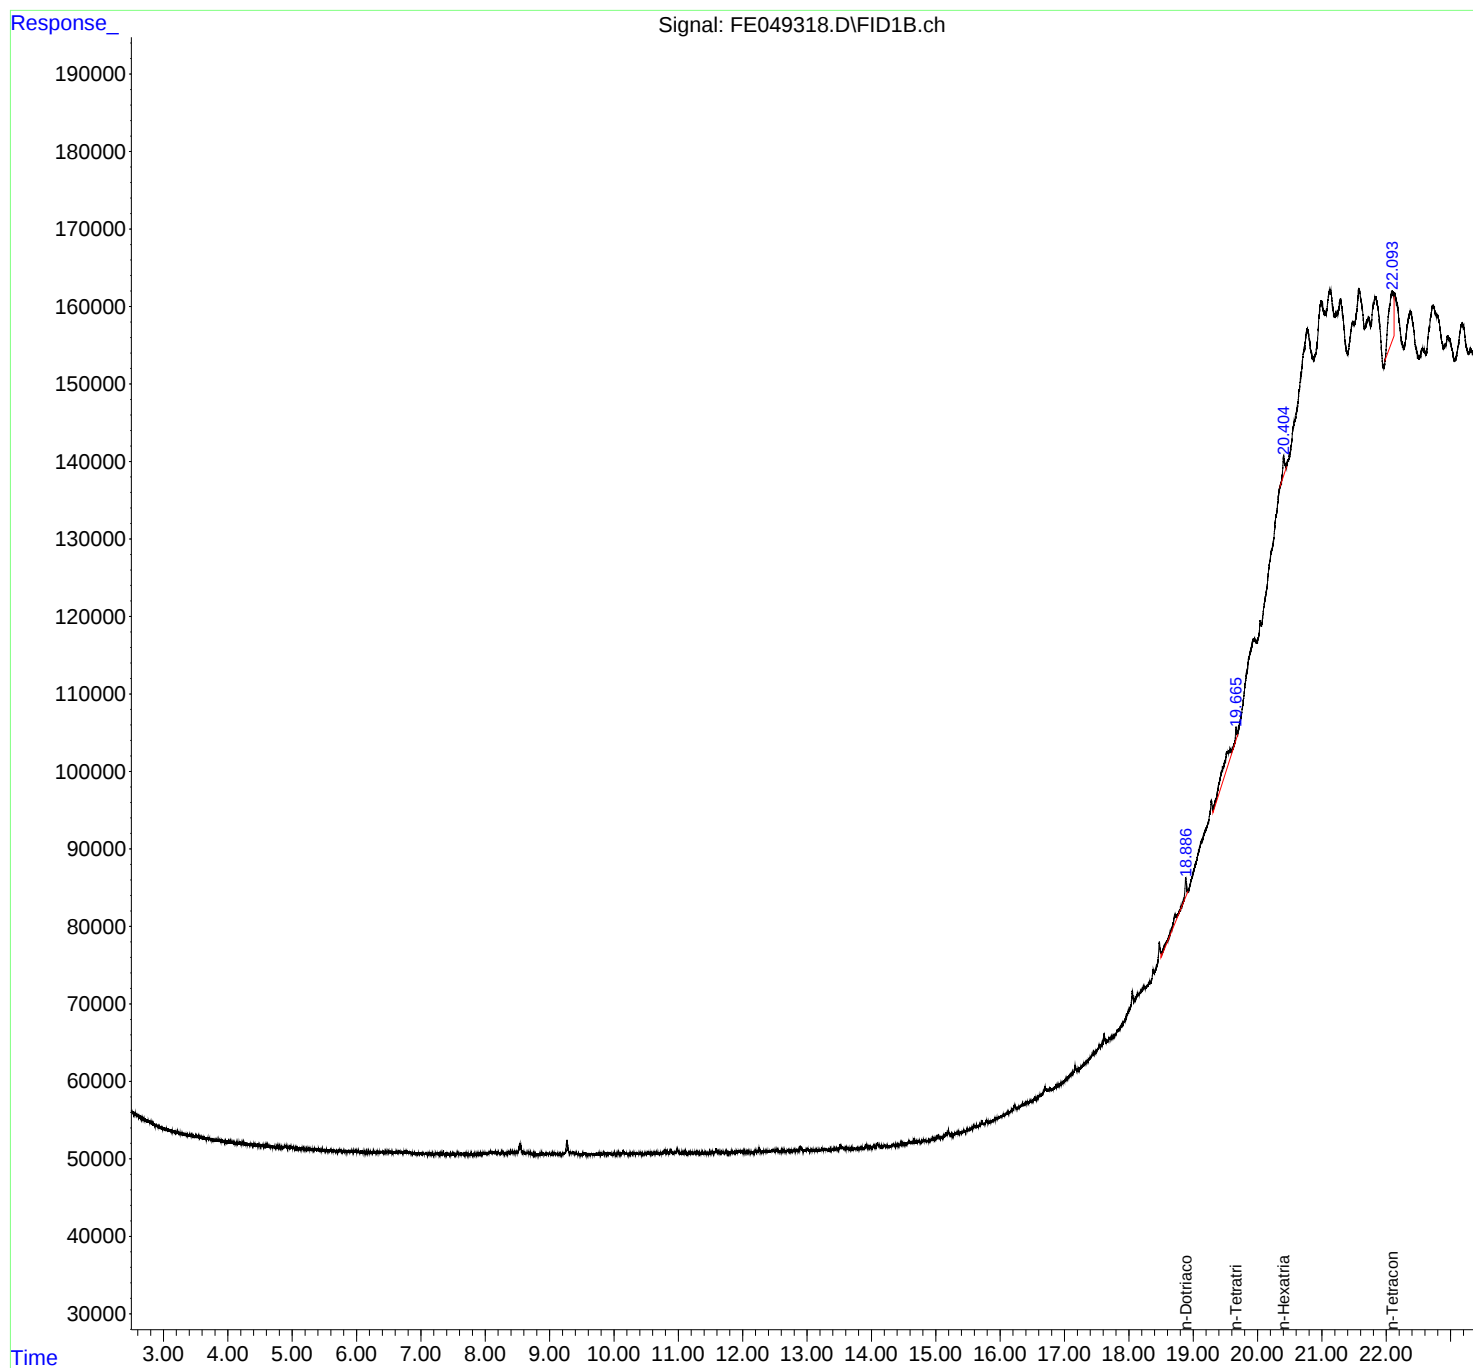


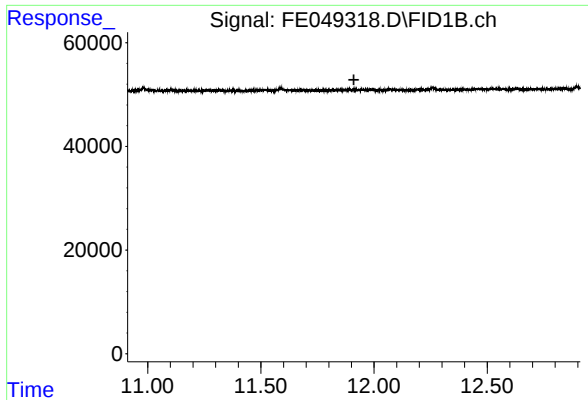

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min  
Exp R.T. : 11.911 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :

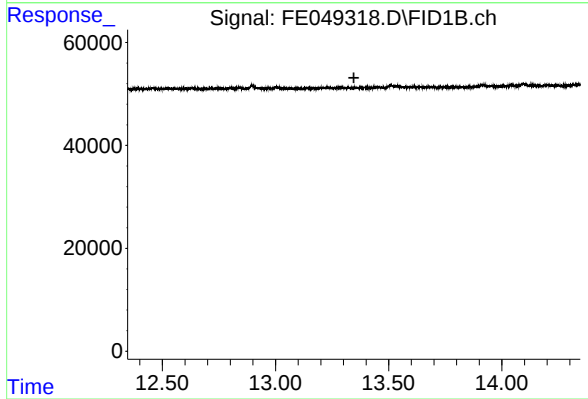


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min  
Exp R.T. : 13.346 min  
Response: 0  
Conc: N.D.

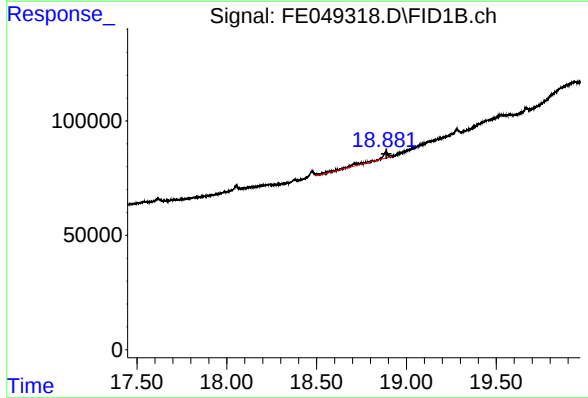


#18 n-Dotriacontane (C32)

R.T.: 18.885 min  
Delta R.T.: -0.003 min  
Response: 101876  
Conc: 0.69 ug/ml

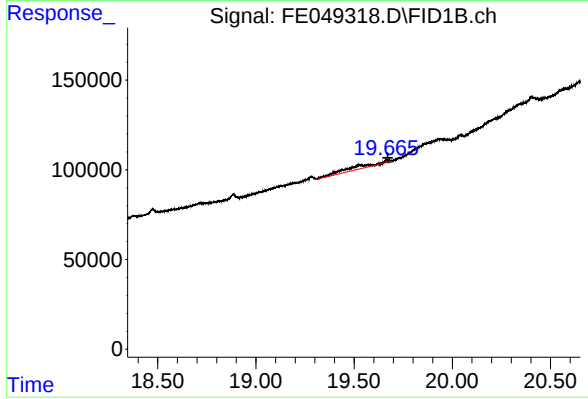

#19 n-Tetratriacontane (C34)

R.T.: 19.668 min  
Delta R.T.: -0.003 min  
Response: 237591  
Conc: 1.63 ug/ml

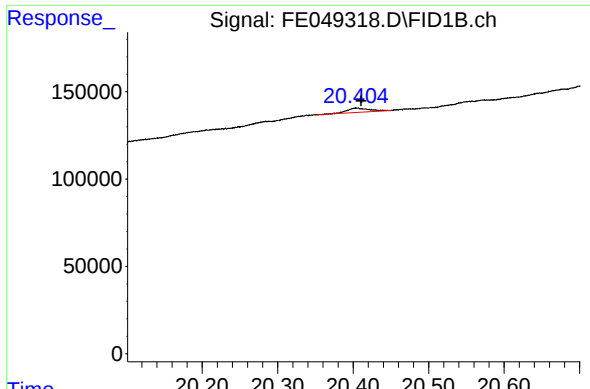


#20 n-Hexatriacontane (C36)

R.T.: 20.405 min  
Delta R.T.: -0.006 min  
Response: 49936  
Conc: 0.35 ug/ml

Instrument :

FID\_E

ClientSampleId :

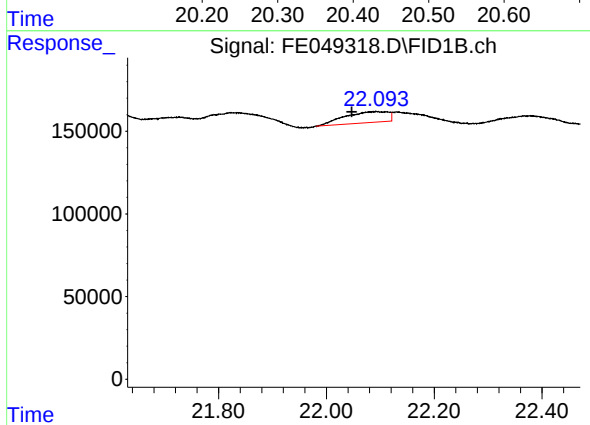

#22 n-Tetracontane (C40)

R.T.: 22.092 min  
Delta R.T.: 0.045 min  
Response: 371506  
Conc: 2.46 ug/ml