

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE073118\
 Data File : FE028445.D
 Signal(s) : FID1B.CH
 Acq On : 01 Aug 2018 11:52
 Operator : AJ\SJ
 Sample : J3762-07
 Misc : FID_E LOD WATER 1 PPB
 ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Aug 01 14:36:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE073118.M
 Quant Title :
 QLast Update : Tue Jul 31 14:21:48 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.985	2530747	15.606 ug/ml
Target Compounds			
2) N-DECANE	4.669	153157	0.829 ug/ml
3) N-DODECANE	6.697	165298	0.834 ug/ml
4) N-TETRADECANE	8.501	171509	0.833 ug/ml
5) N-HEXADECANE	10.110	172986	0.835 ug/ml
6) N-OCTADECANE	11.560	174897	0.857 ug/ml
7) N-EICOSANE	12.875	166320	0.845 ug/ml
8) N-DOCOSANE	14.078	161436	0.849 ug/ml
10) N-TETRACOSANE	15.187	175131	0.943 ug/ml
11) N-HEXACOSANE	16.212	167271	0.915 ug/ml
12) N-OCTACOSANE	17.165	218832	1.188 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE073118\
Data File : FE028445.D
Signal(s) : FID1B.CH
Acq On : 01 Aug 2018 11:52
Operator : AJ\SJ
Sample : J3762-07
Misc : FID_E LOD WATER 1 PPB
ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Aug 01 14:36:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE073118.M
Quant Title :
QLast Update : Tue Jul 31 14:21:48 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

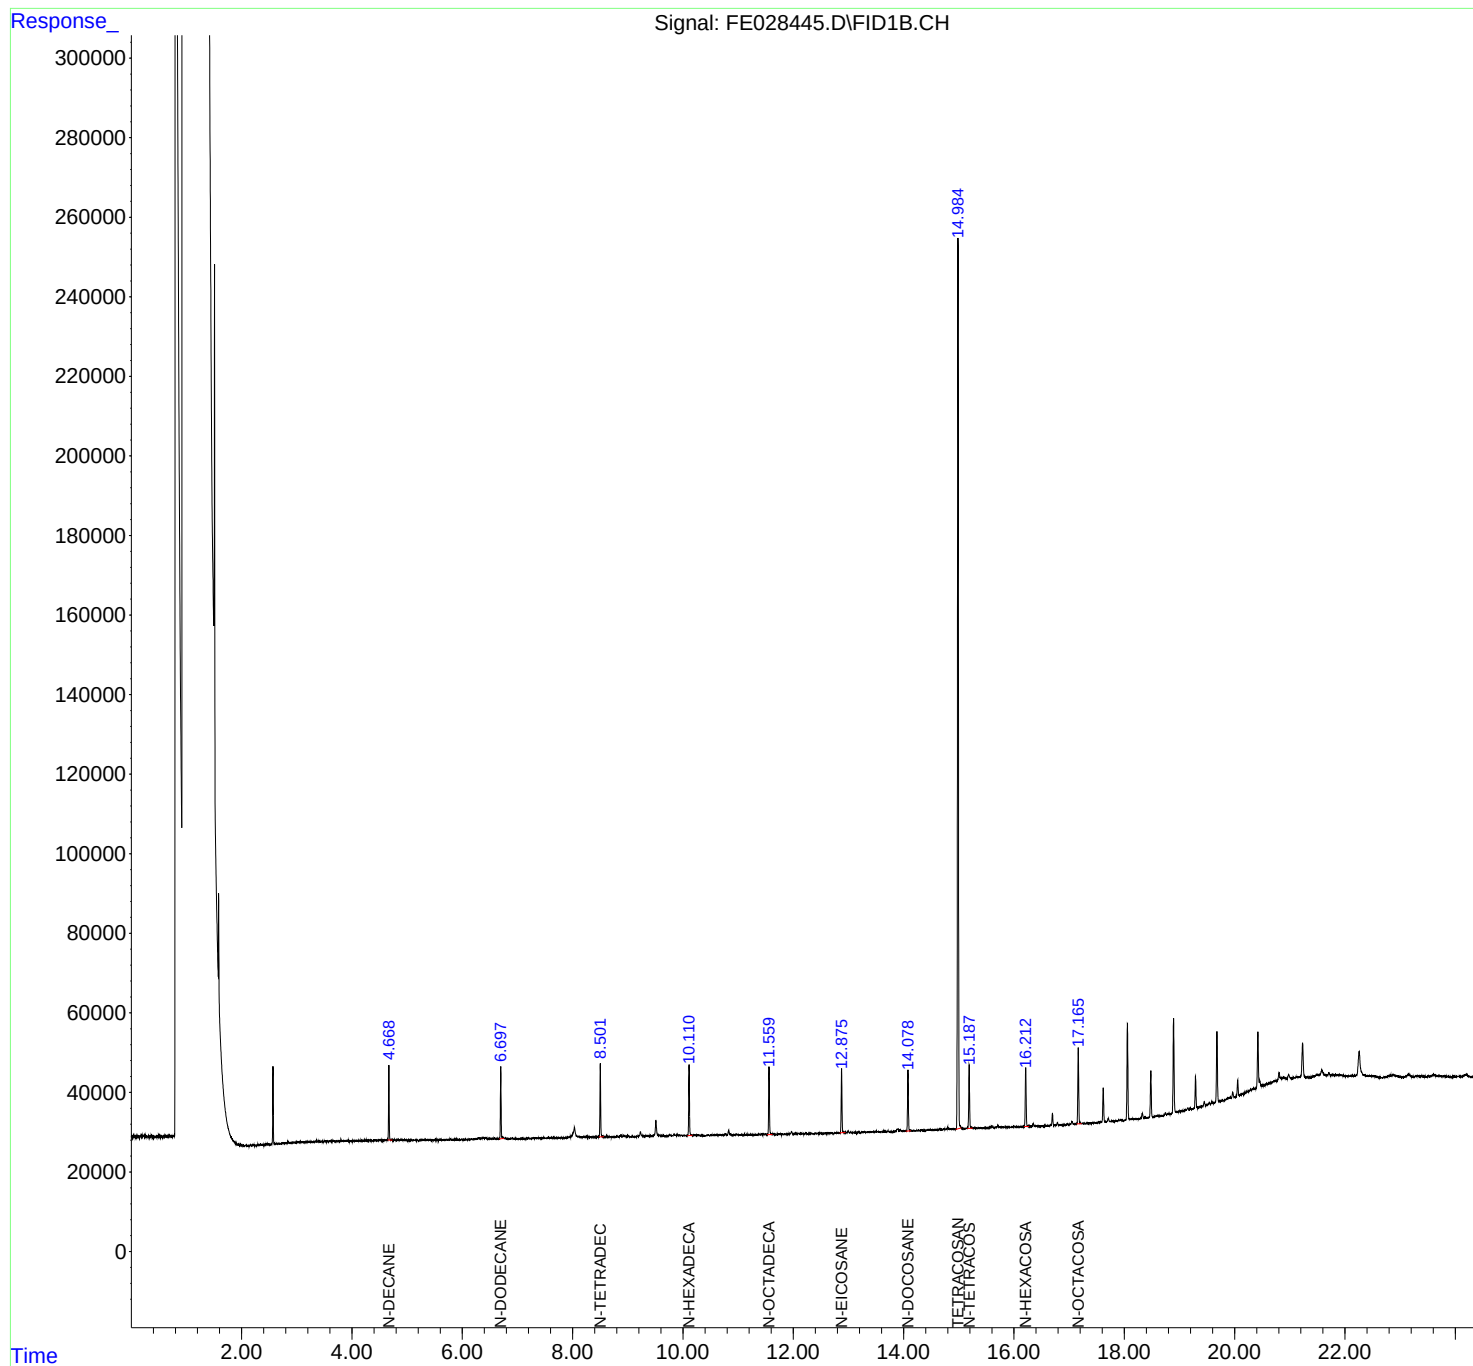

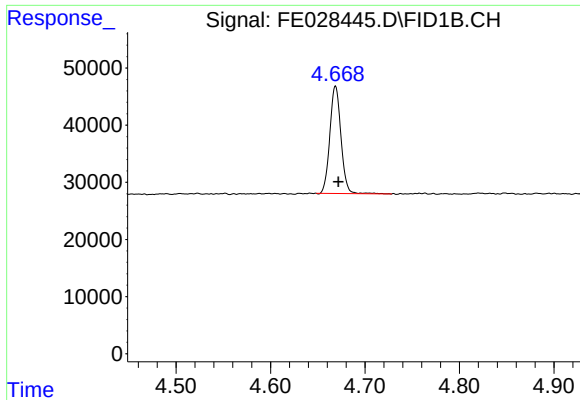


#2 N-DECANE

R.T.: 4.669 min
Delta R.T.: -0.003 min
Response: 153157
Conc: 0.83 ug/ml

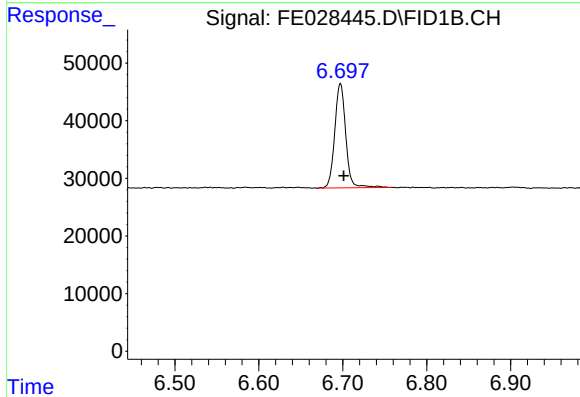


#3 N-DODECANE

R.T.: 6.697 min
Delta R.T.: -0.004 min
Response: 165298
Conc: 0.83 ug/ml

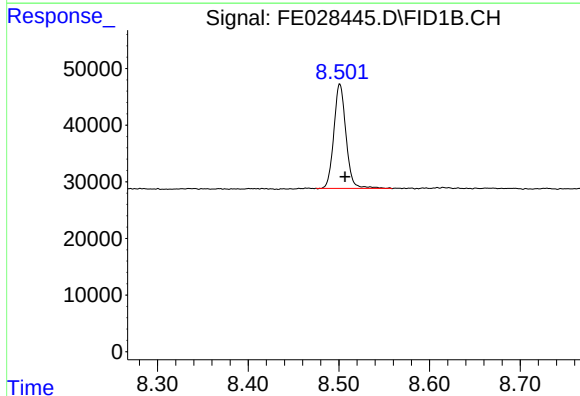


#4 N-TETRADECANE

R.T.: 8.501 min
Delta R.T.: -0.005 min
Response: 171509
Conc: 0.83 ug/ml

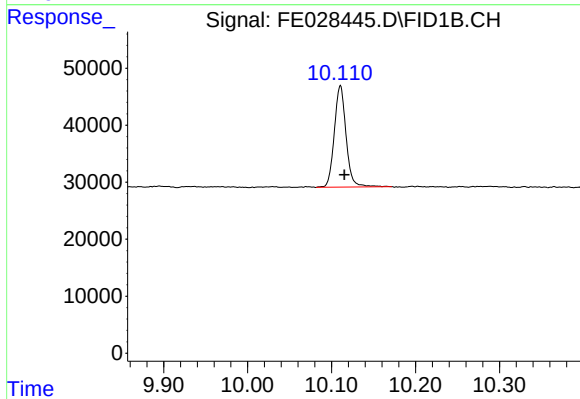


#5 N-HEXADECANE

R.T.: 10.110 min
Delta R.T.: -0.005 min
Response: 172986
Conc: 0.84 ug/ml

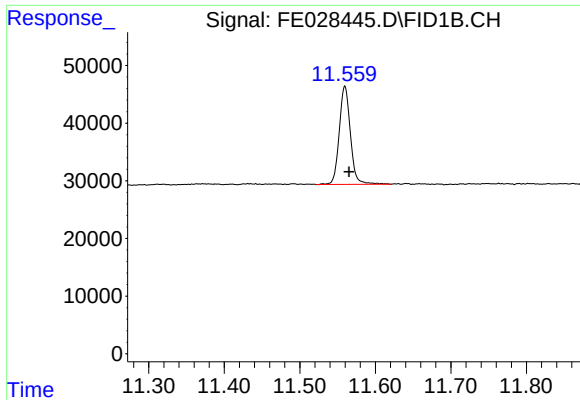


#6 N-OCTADECANE

R.T.: 11.560 min
Delta R.T.: -0.005 min
Response: 174897
Conc: 0.86 ug/ml

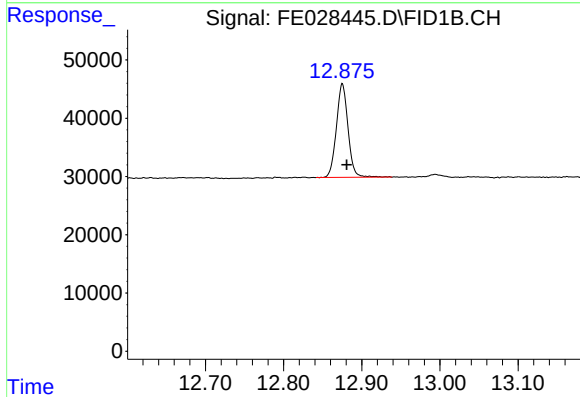


#7 N-EICOSANE

R.T.: 12.875 min
Delta R.T.: -0.006 min
Response: 166320
Conc: 0.84 ug/ml

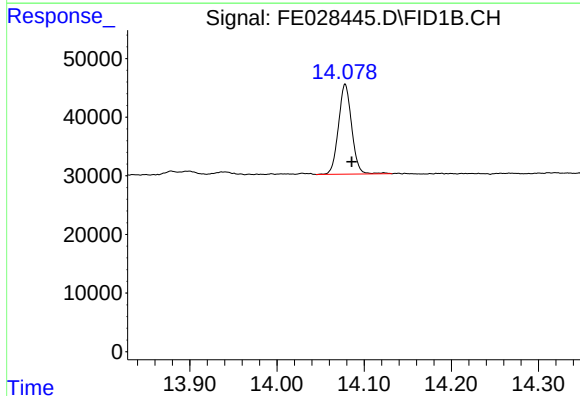


#8 N-DOCOSANE

R.T.: 14.078 min
Delta R.T.: -0.007 min
Response: 161436
Conc: 0.85 ug/ml

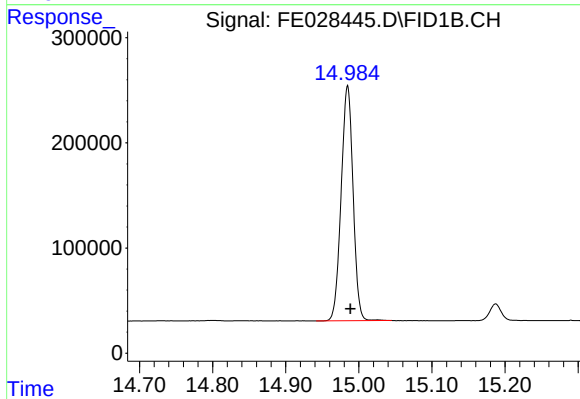


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.985 min
Delta R.T.: -0.004 min
Response: 2530747
Conc: 15.61 ug/ml

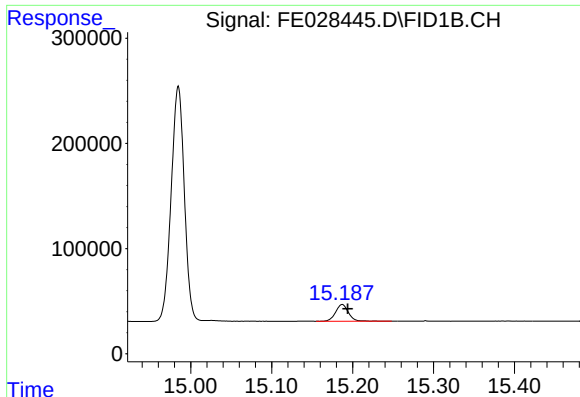


#10 N-TETRACOSANE

R.T.: 15.187 min
Delta R.T.: -0.007 min
Response: 175131
Conc: 0.94 ug/ml

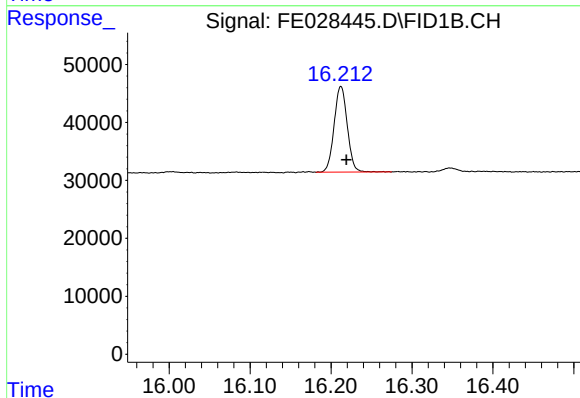

#11 N-HEXACOSANE

R.T.: 16.212 min
Delta R.T.: -0.007 min
Response: 167271
Conc: 0.91 ug/ml

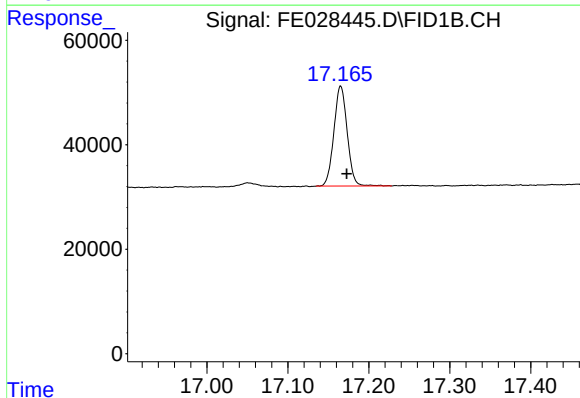

#12 N-OCTACOSANE

R.T.: 17.165 min
Delta R.T.: -0.007 min
Response: 218832
Conc: 1.19 ug/ml