

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE073123AL\
Data File : FE043628.D
Signal(s) : FID1B.ch
Acq On : 31 Jul 2023 10:00
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 31 12:04:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071323.M
Quant Title : GC Extractables
QLast Update : Thu Jul 13 03:02:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	n-Tetratriacontane (C34)	19.718	186291	1.291 ug/ml
21) T	n-Octatriacontane (C38)	21.154	654121	4.585 ug/ml
22) T	n-Tetracontane (C40)	22.117	94779	0.642 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE073123AL\
Data File : FE043628.D
Signal(s) : FID1B.ch
Acq On : 31 Jul 2023 10:00
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 31 12:04:14 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071323.M
Quant Title : GC Extractables
QLast Update : Thu Jul 13 03:02:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

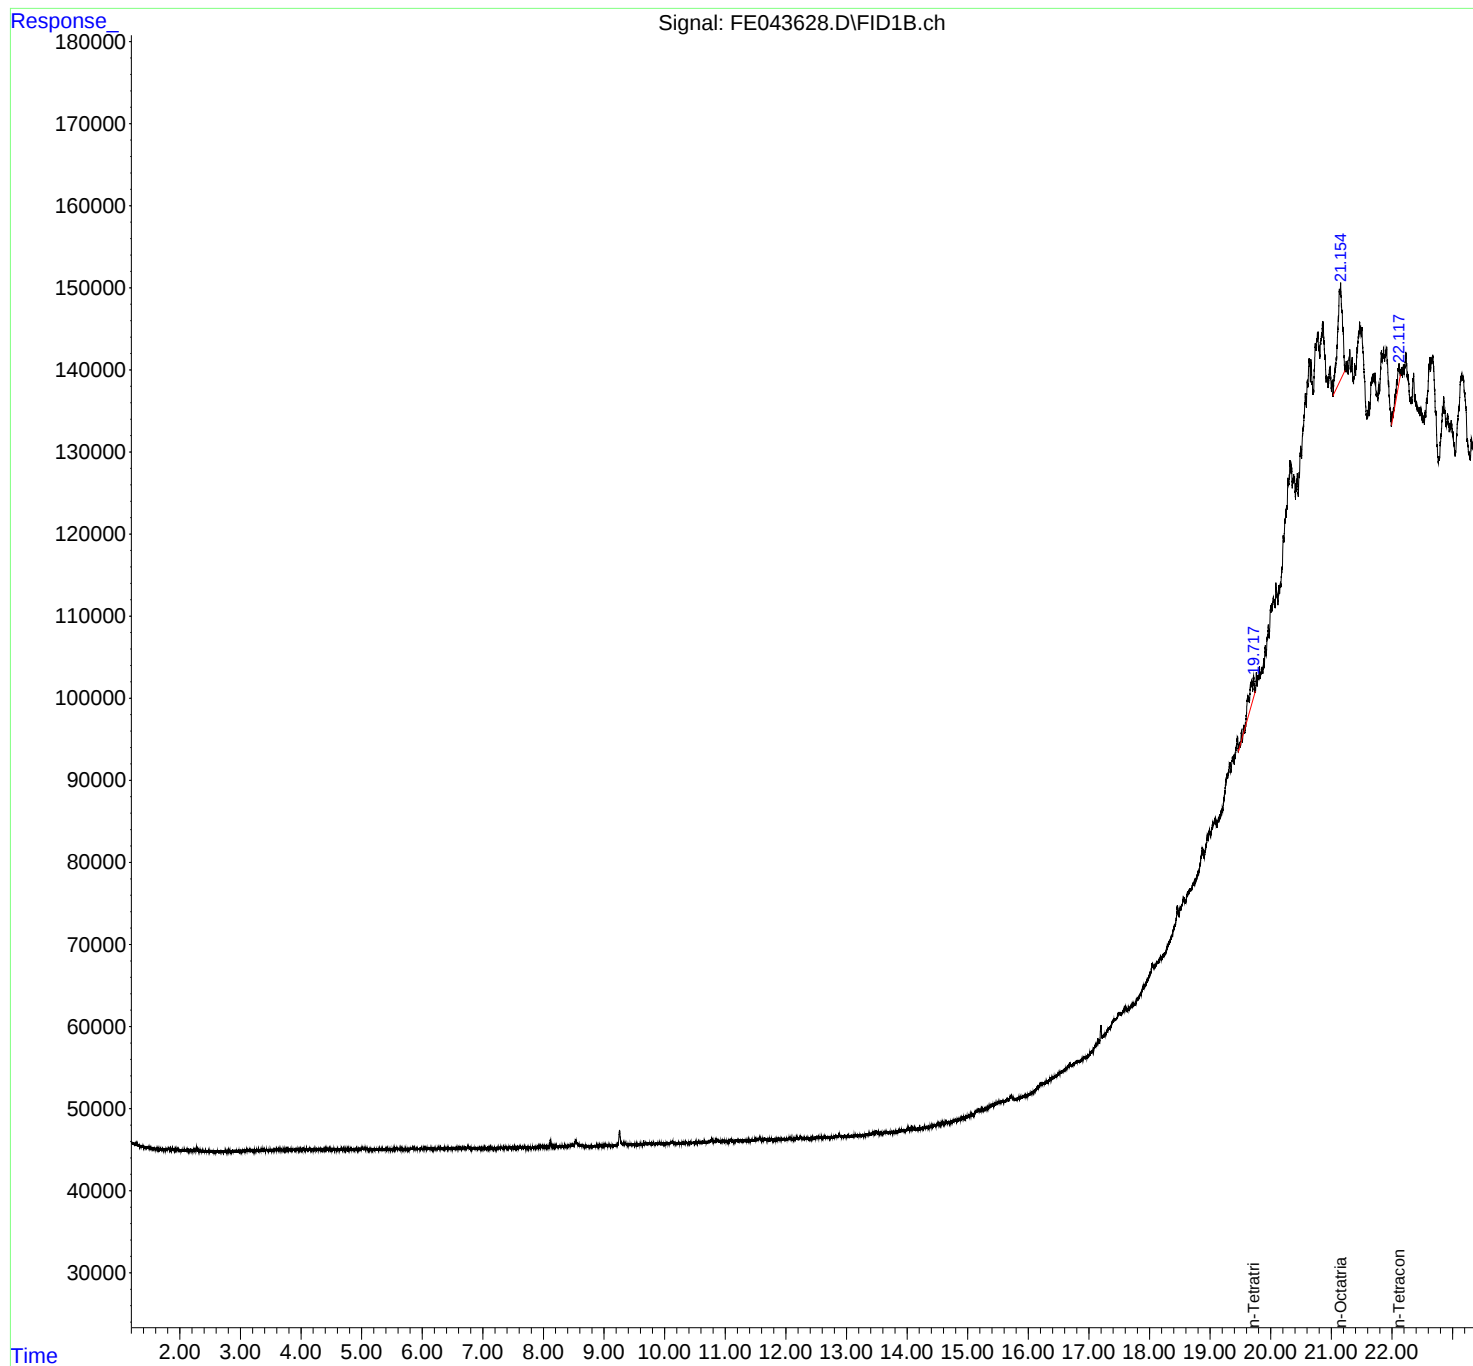


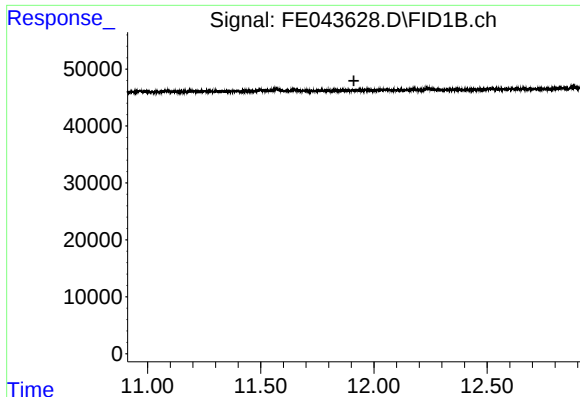

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.911 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

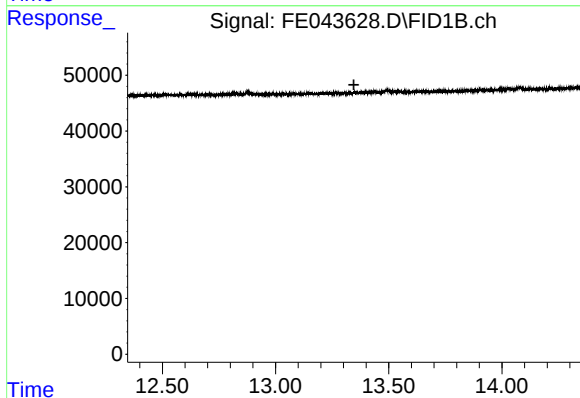


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.346 min
Response: 0
Conc: N.D.

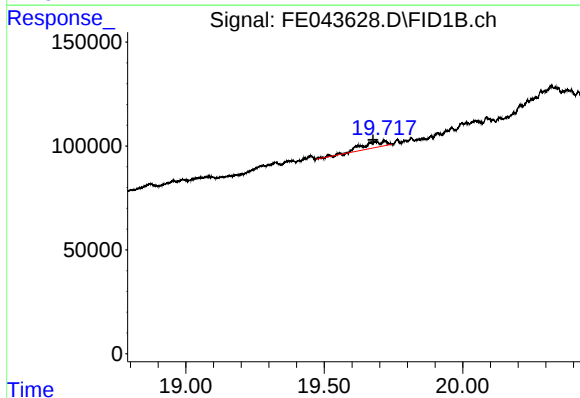


#19 n-Tetratriacontane (C34)

R.T.: 19.718 min
Delta R.T.: 0.042 min
Response: 186291
Conc: 1.29 ug/ml

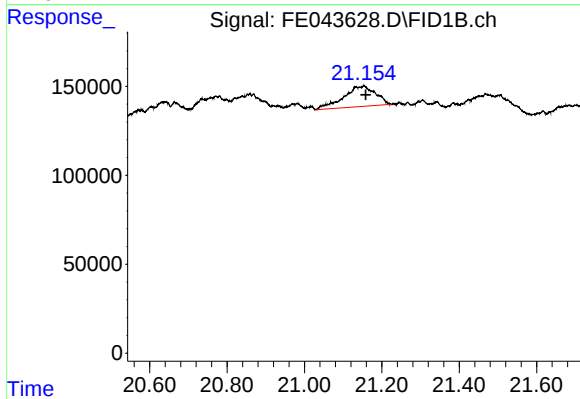

#21 n-Octatriacontane (C38)

R.T.: 21.154 min
Delta R.T.: -0.004 min
Response: 654121
Conc: 4.59 ug/ml

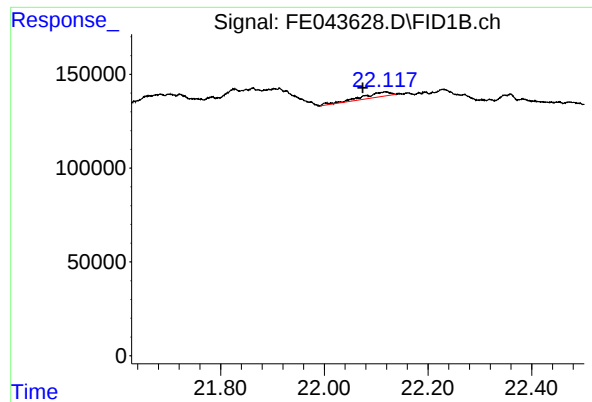

#22 n-Tetracontane (C40)

R.T.: 22.117 min
Delta R.T.: 0.043 min
Response: 94779
Conc: 0.64 ug/ml

Instrument :

FID_E

ClientSampleId :