

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE073123AL\
 Data File : FE043652.D
 Signal(s) : FID1B.ch
 Acq On : 31 Jul 2023 22:45
 Operator : YP\AJ
 Sample : 03835-01DL 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 HR-01-072823DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 08/01/2023
 Supervised By :Ankita Jodhani 08/01/2023

Integration File: autoint1.e
 Quant Time: Aug 01 04:09:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071323.M
 Quant Title : GC Extractables
 QLast Update : Thu Jul 13 03:02:53 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.882	320051	1.787 ug/ml
Spiked Amount 50.000		Recovery =	3.57%
12) S 1-chlorooctadecane (S...	13.316	486900	3.706 ug/mlm
Spiked Amount 50.000		Recovery =	7.41%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE073123AL\
Data File : FE043652.D
Signal(s) : FID1B.ch
Acq On : 31 Jul 2023 22:45
Operator : YP\AJ
Sample : 03835-01DL 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
HR-01-072823DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2023
Supervised By :Ankita Jodhani 08/01/2023

Integration File: autoint1.e
Quant Time: Aug 01 04:09:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071323.M
Quant Title : GC Extractables
QLast Update : Thu Jul 13 03:02:53 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

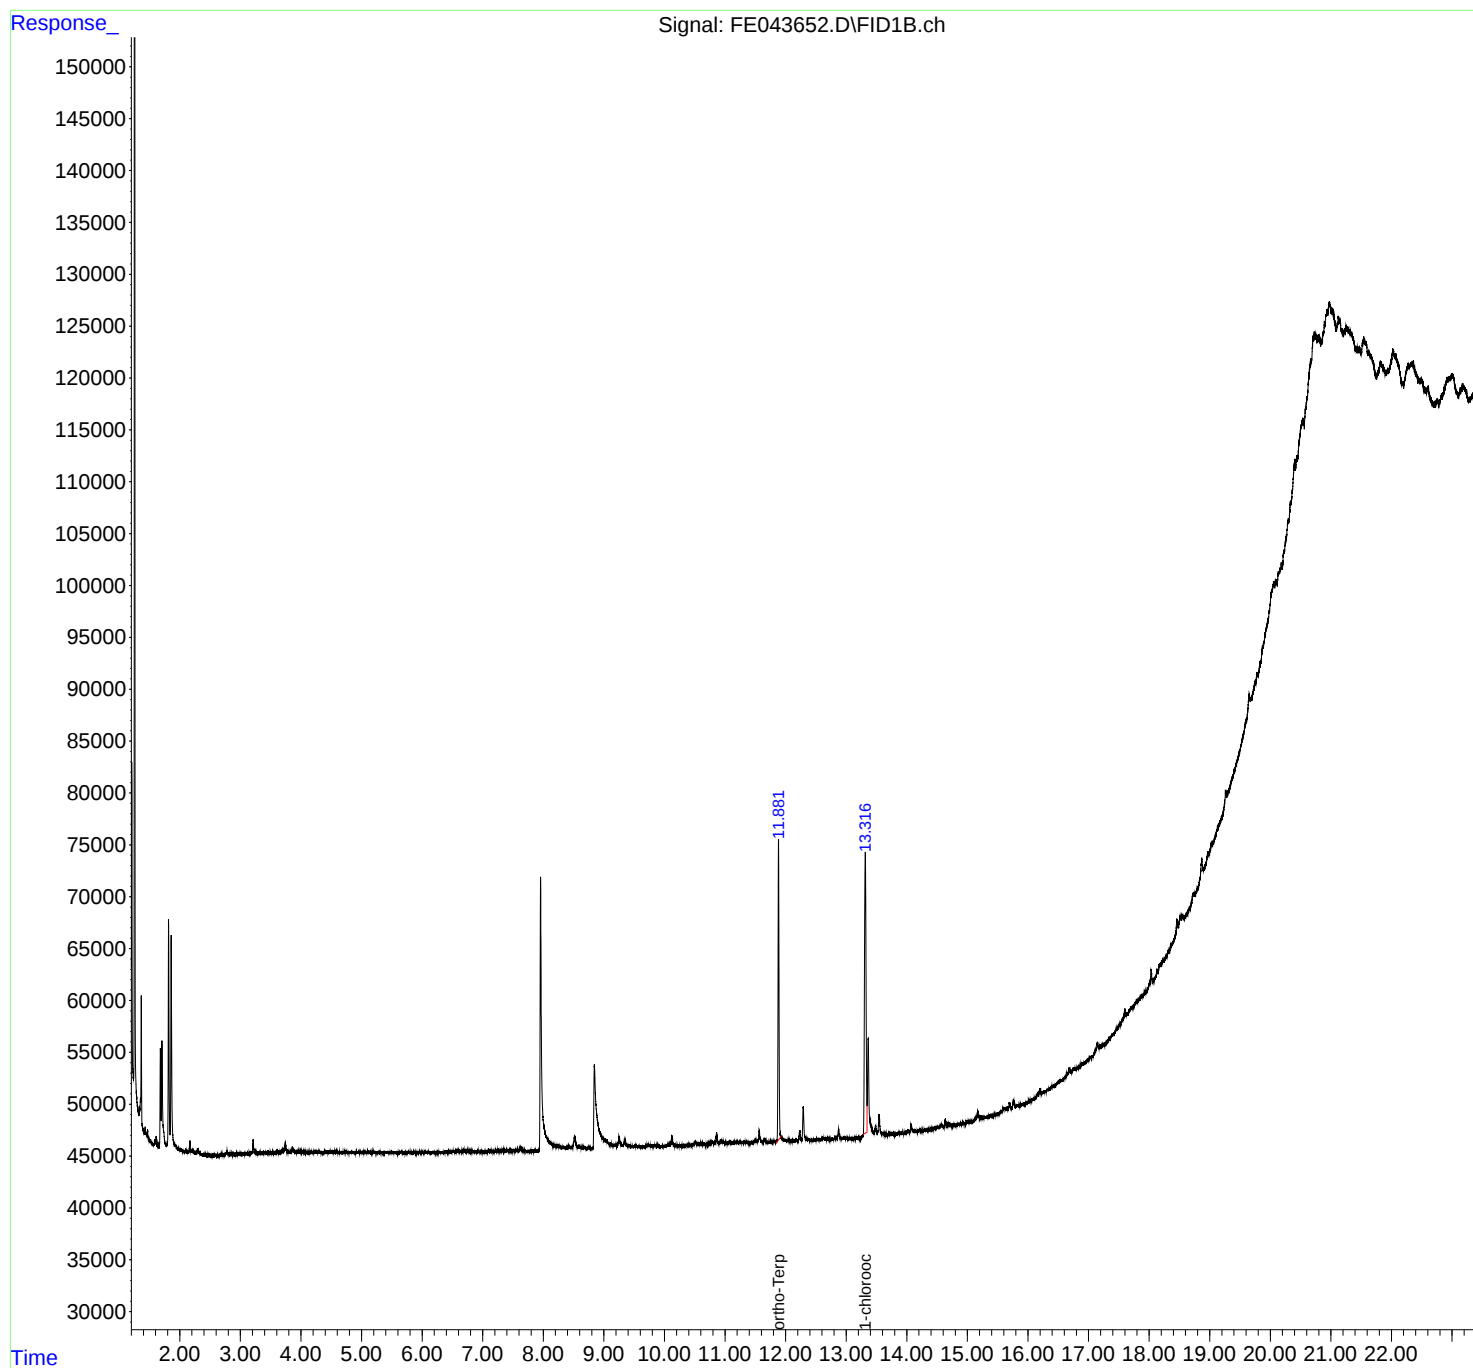

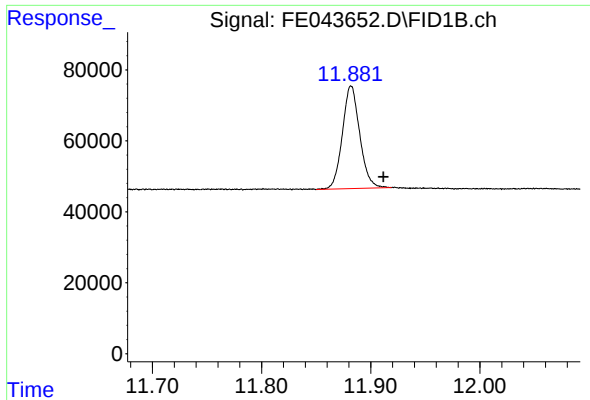


#9 ortho-Terphenyl (SURR)

R.T.: 11.882 min
Delta R.T.: -0.029 min
Response: 320051
Conc: 1.79 ug/ml

Instrument :
FID_E
ClientSampleId :
HR-01-072823DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/01/2023
Supervised By :Ankita Jodhani 08/01/2023

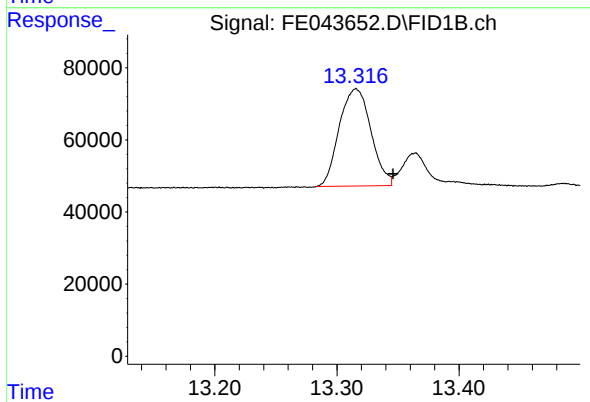

#12 1-chlorooctadecane (SURR)

R.T.: 13.316 min
Delta R.T.: -0.030 min
Response: 486900
Conc: 3.71 ug/ml m