

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE080125AL\  
 Data File : FE055117.D  
 Signal(s) : FID1B.ch  
 Acq On : 01 Aug 2025 20:08  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 I.BLK

Integration File: autoint1.e  
 Quant Time: Aug 02 01:31:16 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 080125.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Aug 01 13:47:09 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

#### System Monitoring Compounds

##### Target Compounds

|       |                          |         |        |             |
|-------|--------------------------|---------|--------|-------------|
| 15) T | n-Hexacosane (C26)       | 16.406  | 38200  | 0.319 ug/ml |
| 16) T | n-Octacosane (C28)       | 17.361  | 41329  | 0.348 ug/ml |
| 17) T | n-Tricontane (C30)       | 18.249  | 131448 | 1.068 ug/ml |
| 18) T | n-Dotriacontane (C32)    | 19.083  | 183250 | 1.502 ug/ml |
| 19) T | n-Tetratriacontane (C34) | 19.870  | 89983  | 0.770 ug/ml |
| 20) T | n-Hexatriacontane (C36)  | 20.610  | 51293  | 0.469 ug/ml |
| 22) T | n-Tetracontane (C40)     | 22.446f | 32104  | 0.307 ug/ml |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE080125AL\  
Data File : FE055117.D  
Signal(s) : FID1B.ch  
Acq On : 01 Aug 2025 20:08  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
I.BLK

Integration File: autoint1.e  
Quant Time: Aug 02 01:31:16 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 080125.M  
Quant Title : GC Extractables  
QLast Update : Fri Aug 01 13:47:09 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

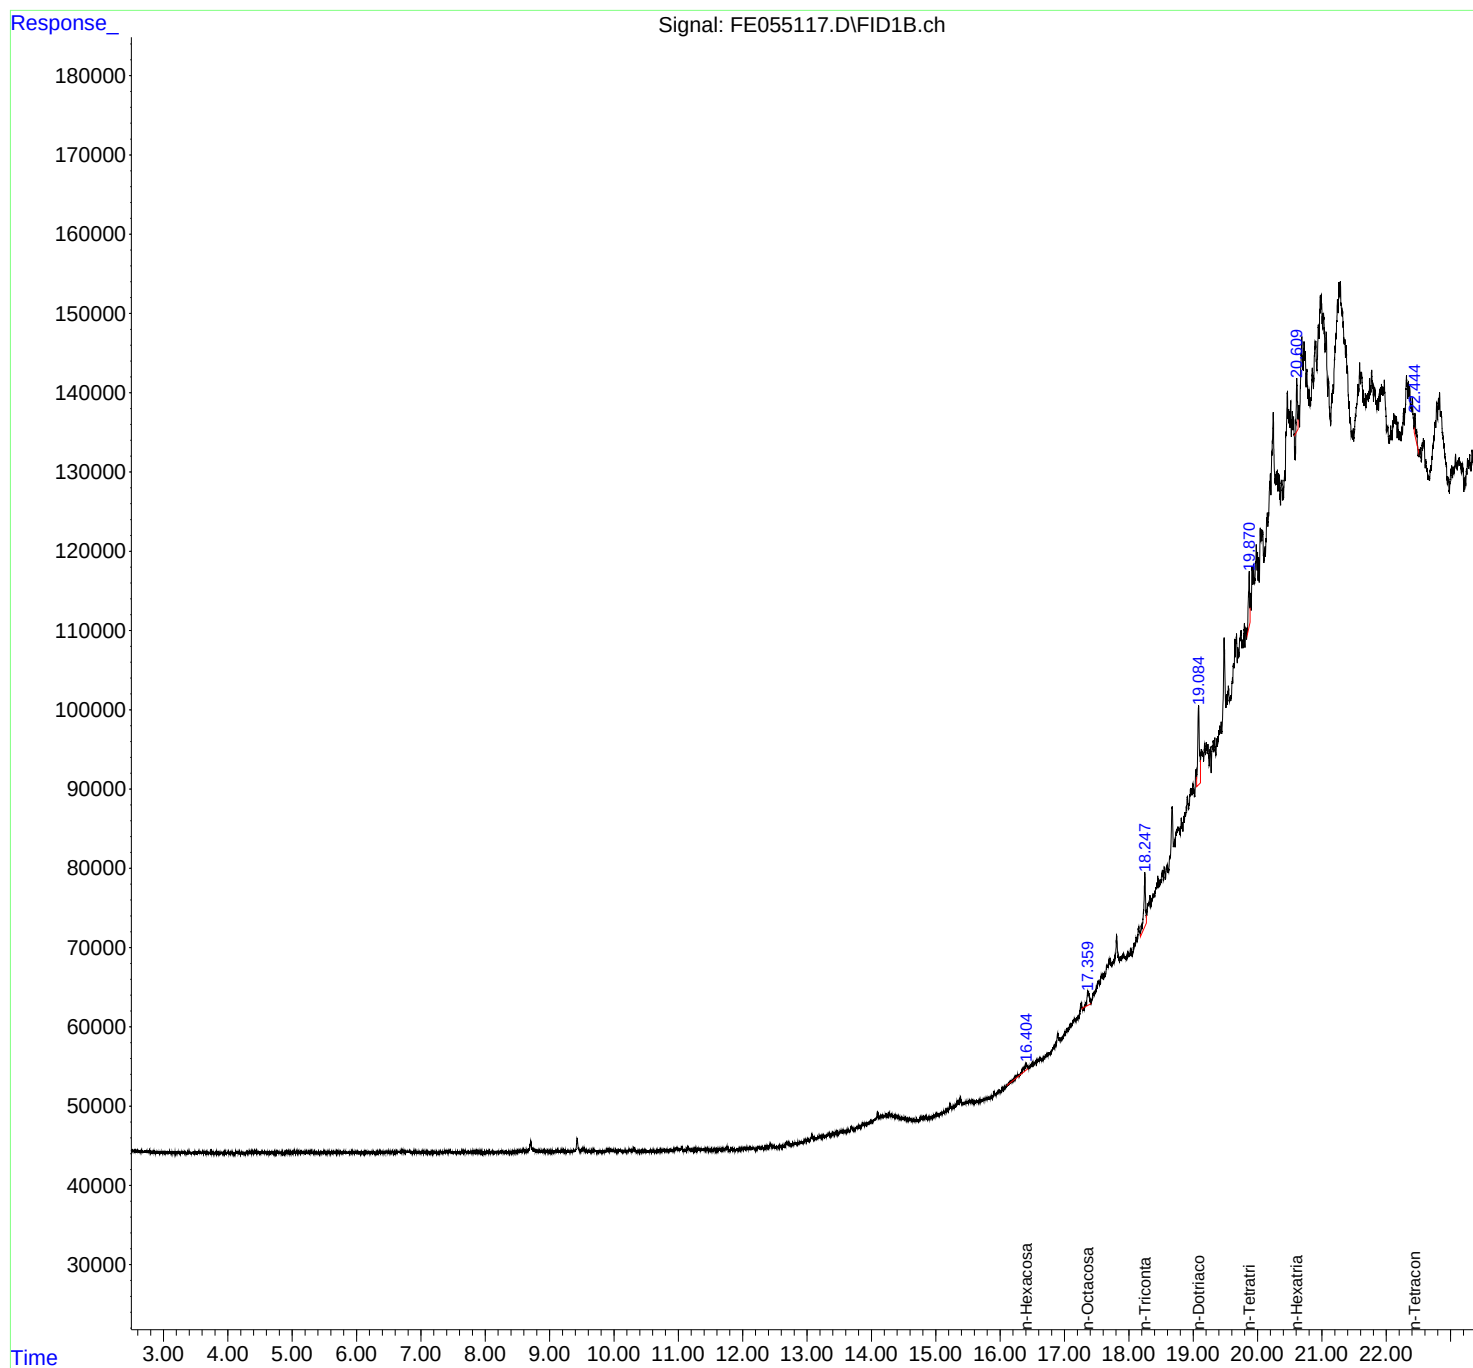


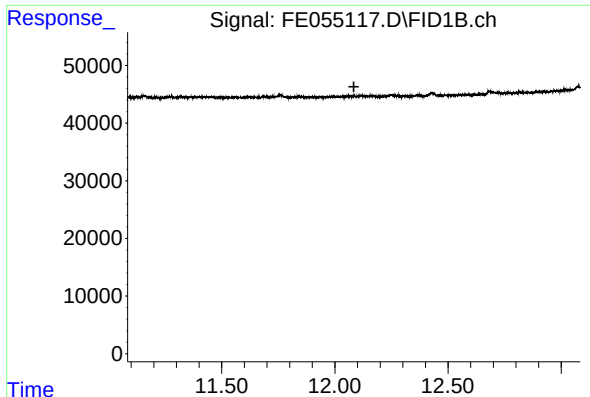

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min  
Exp R.T.: 12.084 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :  
I.BLK

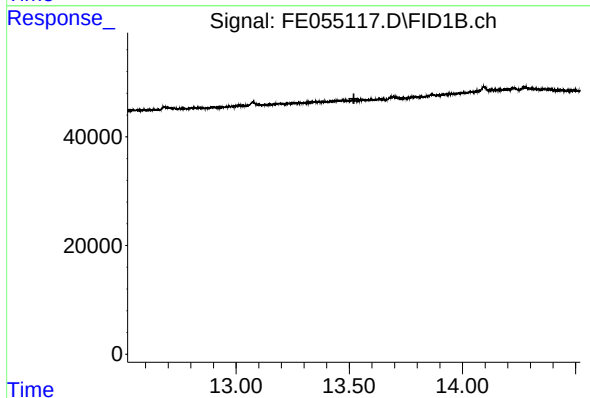


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min  
Exp R.T.: 13.520 min  
Response: 0  
Conc: N.D.

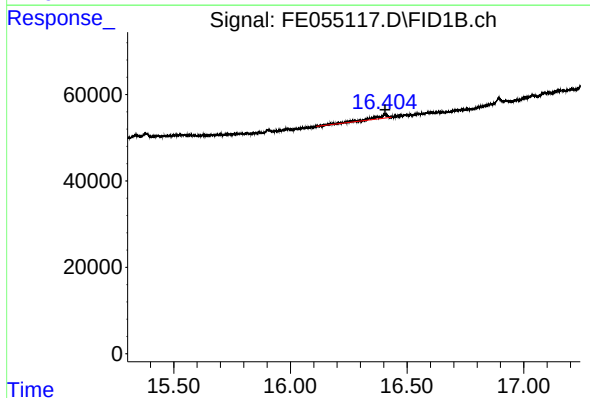


#15 n-Hexacosane (C26)

R.T.: 16.406 min  
Delta R.T.: 0.000 min  
Response: 38200  
Conc: 0.32 ug/ml

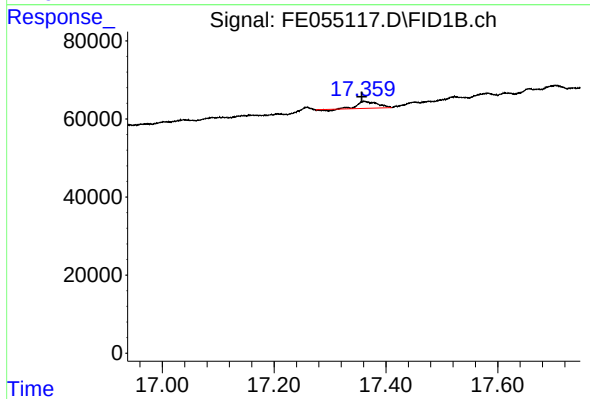

#16 n-Octacosane (C28)


R.T.: 17.361 min  
Delta R.T.: 0.004 min  
Response: 41329  
Conc: 0.35 ug/ml

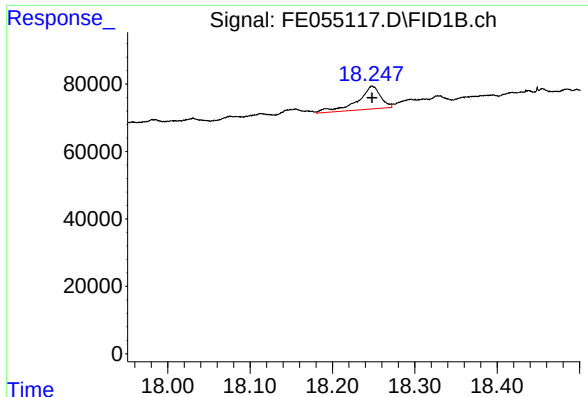

#17 n-Tricontane (C30)


R.T.: 18.249 min  
Delta R.T.: 0.000 min  
Response: 131448  
Conc: 1.07 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
I.BLK

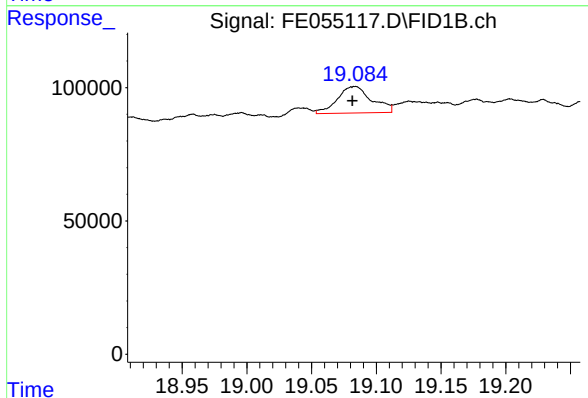


#18 n-Dotriacontane (C32)

R.T.: 19.083 min  
Delta R.T.: 0.001 min  
Response: 183250  
Conc: 1.50 ug/ml

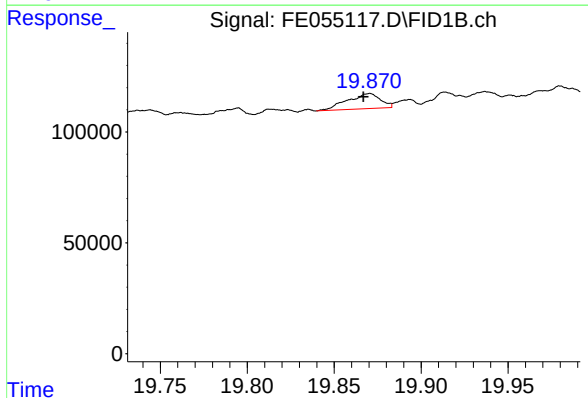


#19 n-Tetratriacontane (C34)

R.T.: 19.870 min  
Delta R.T.: 0.003 min  
Response: 89983  
Conc: 0.77 ug/ml

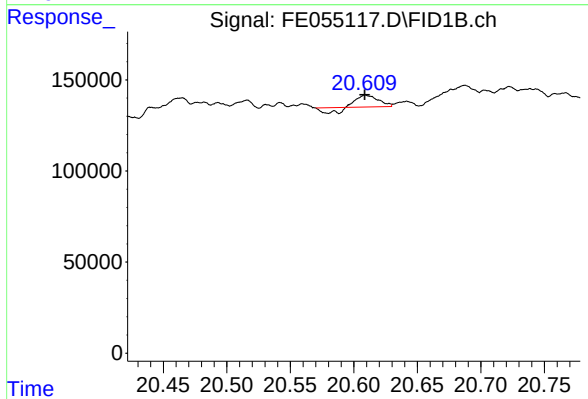

#20 n-Hexatriacontane (C36)

R.T.: 20.610 min  
Delta R.T.: 0.001 min  
Response: 51293  
Conc: 0.47 ug/ml

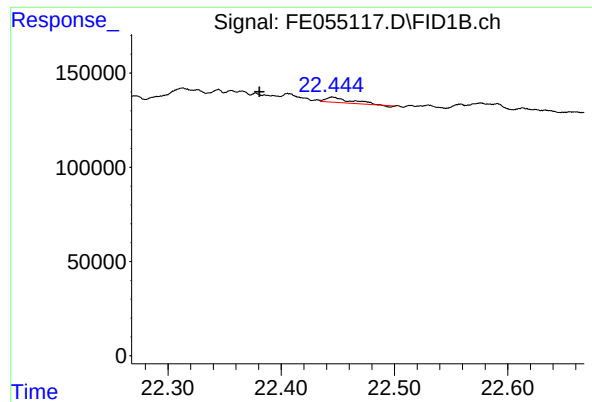

#22 n-Tetracontane (C40)

R.T.: 22.446 min  
Delta R.T.: 0.065 min  
Response: 32104  
Conc: 0.31 ug/ml

Instrument :

FID\_E

ClientSampleId :

I.BLK