

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080222AL\
 Data File : FE036811.D
 Signal(s) : FID1B.ch
 Acq On : 02 Aug 2022 08:18
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 03 03:34:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071722.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 18 02:35:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

14) T	n-Tetracosane (C24)	15.103	376914	2.211 ug/ml
17) T	n-Tricontane (C30)	17.991	97577	<MDL ug/ml
18) T	n-Dotriacontane (C32)	18.824	164024	1.364 ug/ml
19) T	n-Tetratriacontane (C34)	19.608	196386	2.358 ug/ml
20) T	n-Hexatriacontane (C36)	20.351	758020	12.910 ug/ml
21) T	n-Octatriacontane (C38)	21.073	575433	11.477 ug/ml
22) T	n-Tetracontane (C40)	21.957	899628	17.420 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080222AL\
Data File : FE036811.D
Signal(s) : FID1B.ch
Acq On : 02 Aug 2022 08:18
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 03 03:34:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071722.M
Quant Title : GC Extractables
QLast Update : Mon Jul 18 02:35:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

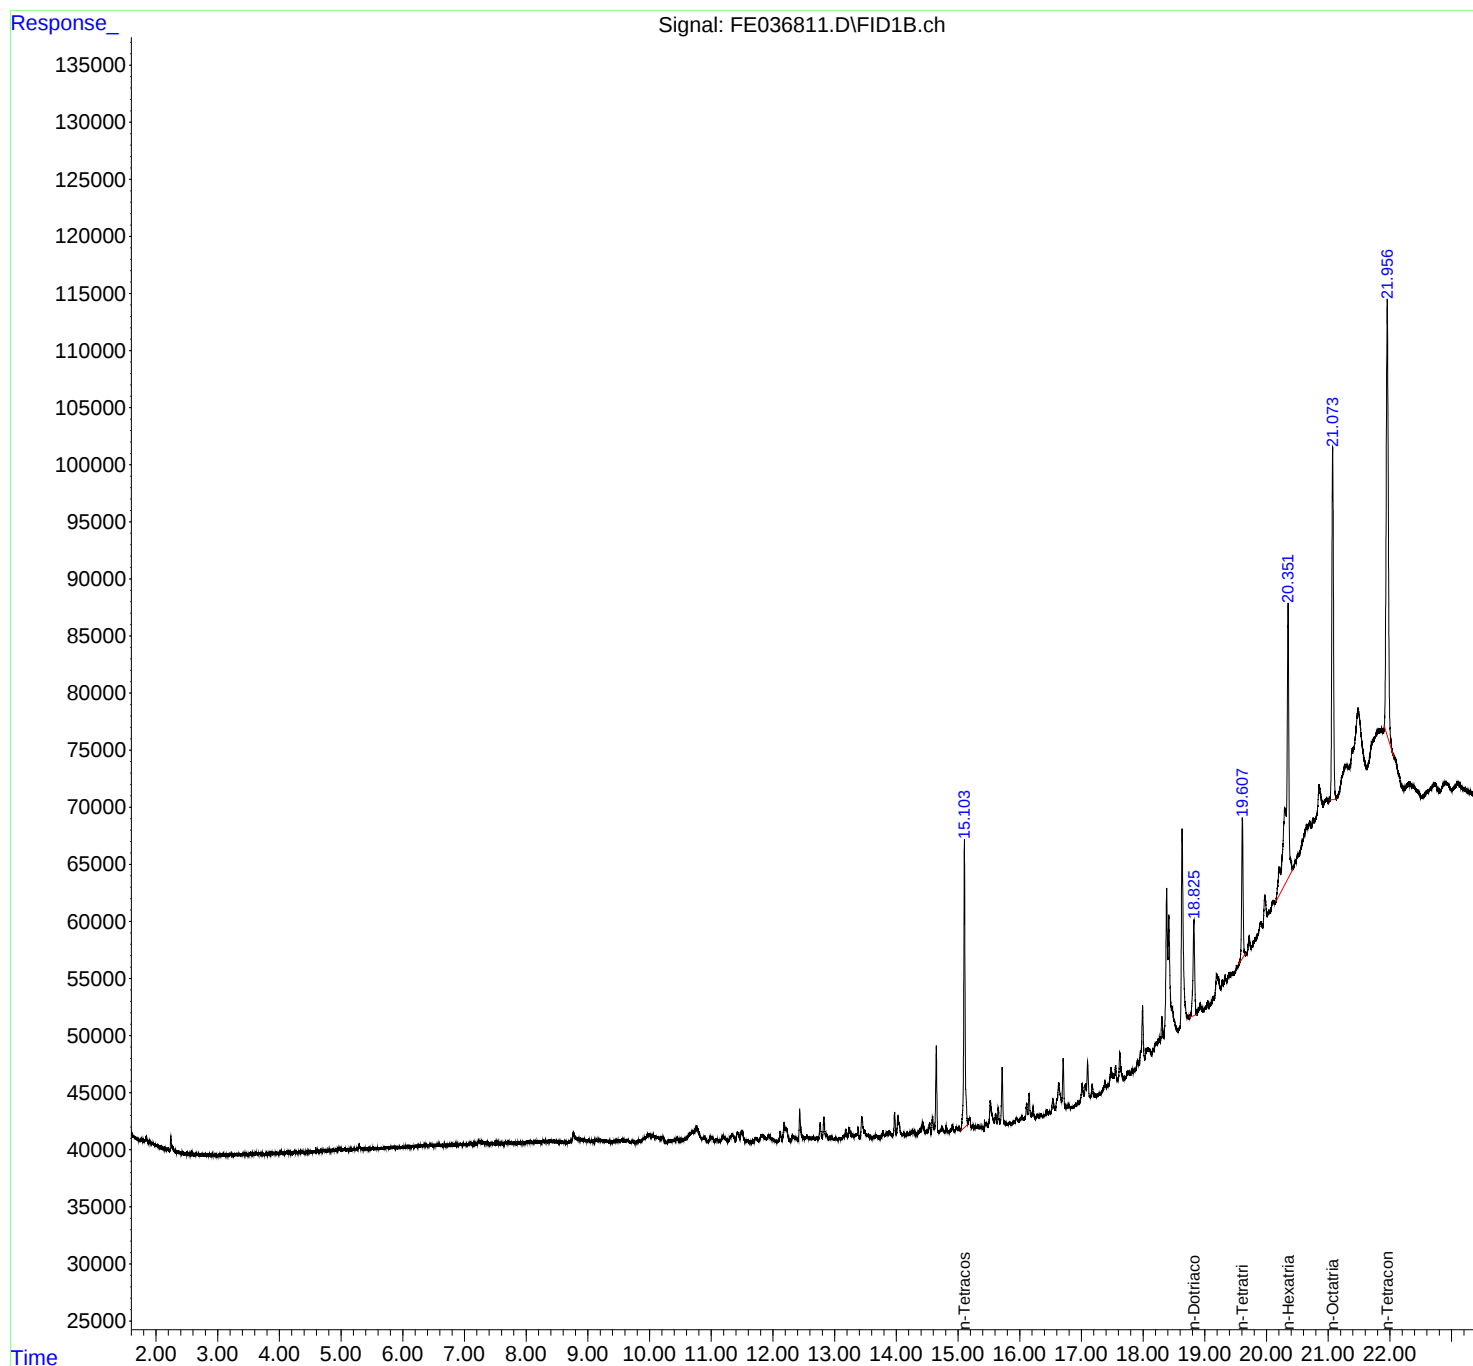


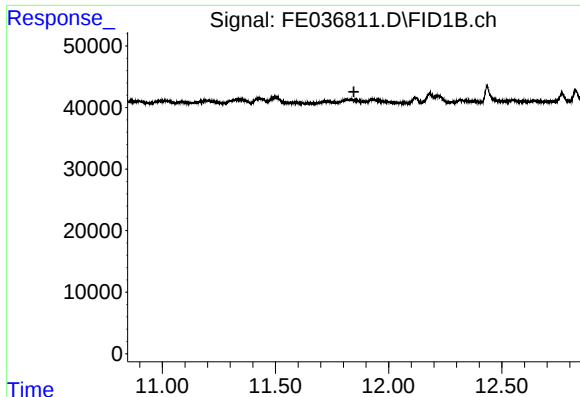

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.846 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

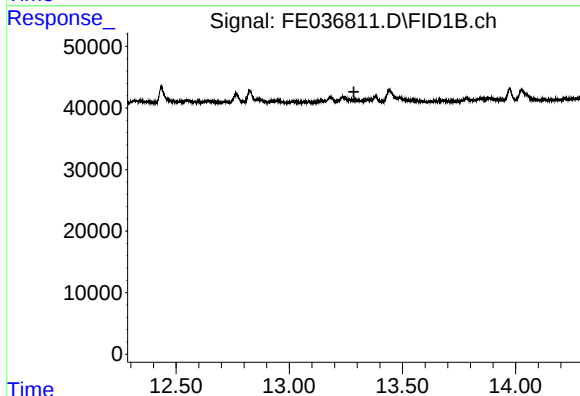


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.286 min
Response: 0
Conc: N.D.

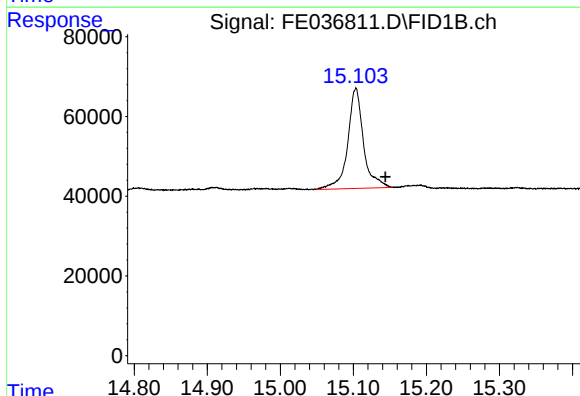


#14 n-Tetracosane (C24)

R.T.: 15.103 min
Delta R.T.: -0.040 min
Response: 376914
Conc: 2.21 ug/ml

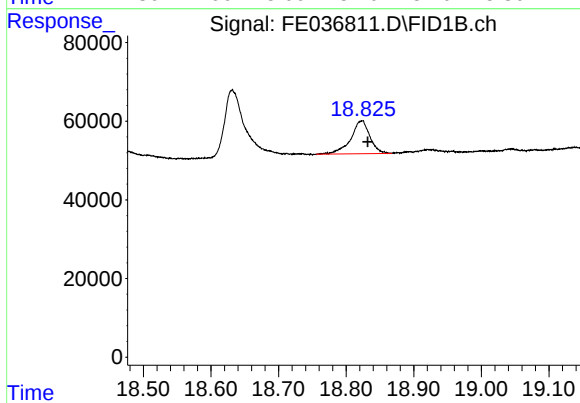

#18 n-Dotriacontane (C32)


R.T.: 18.824 min
Delta R.T.: -0.008 min
Response: 164024
Conc: 1.36 ug/ml

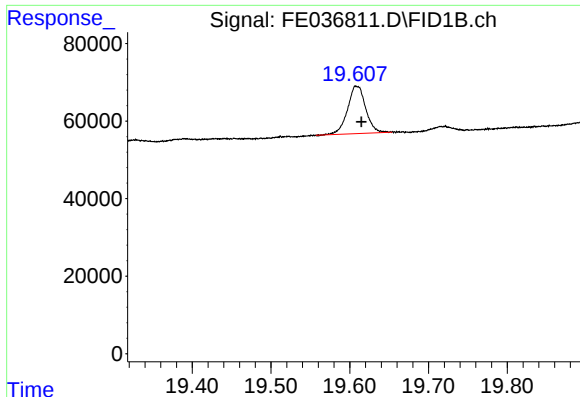

#19 n-Tetratriacontane (C34)


R.T.: 19.608 min
Delta R.T.: -0.006 min
Response: 196386
Conc: 2.36 ug/ml

Instrument :
FID_E
ClientSampleId :

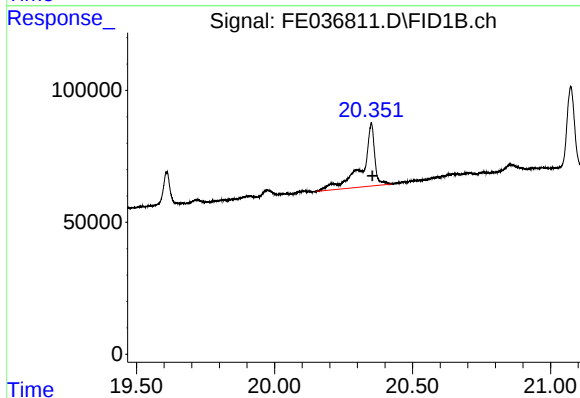


#20 n-Hexatriacontane (C36)

R.T.: 20.351 min
Delta R.T.: -0.003 min
Response: 758020
Conc: 12.91 ug/ml

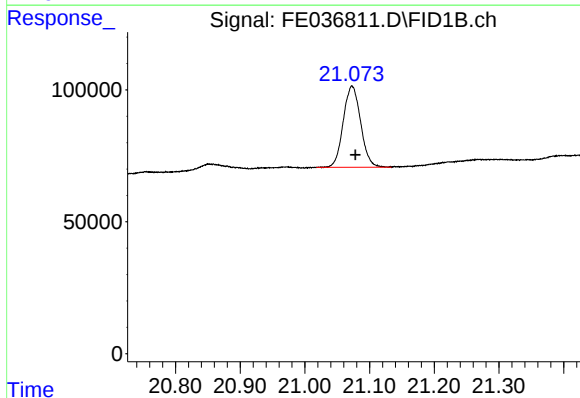

#21 n-Octatriacontane (C38)

R.T.: 21.073 min
Delta R.T.: -0.005 min
Response: 575433
Conc: 11.48 ug/ml

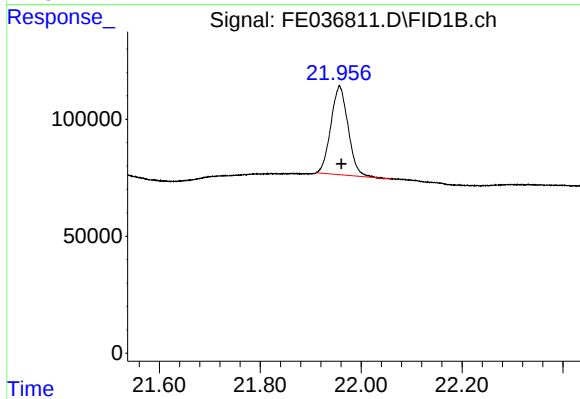

#22 n-Tetracontane (C40)

R.T.: 21.957 min
Delta R.T.: -0.003 min
Response: 899628
Conc: 17.42 ug/ml