

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080224\
Data File : FE049406.D
Signal(s) : FID1B.ch
Acq On : 02 Aug 2024 21:21
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 03 03:22:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072924.M
Quant Title :
QLast Update : Tue Jul 30 04:50:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.877	107751	0.767 ug/ml
16)	N-HEXATRIACONTANE	20.454	109792	1.072 ug/ml
17)	N-OCTATRIACONTANE	21.144	171261	1.815 ug/ml
18)	N-TETRACONTANE	22.092	446073	4.713 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080224\
Data File : FE049406.D
Signal(s) : FID1B.ch
Acq On : 02 Aug 2024 21:21
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 03 03:22:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072924.M
Quant Title :
QLast Update : Tue Jul 30 04:50:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

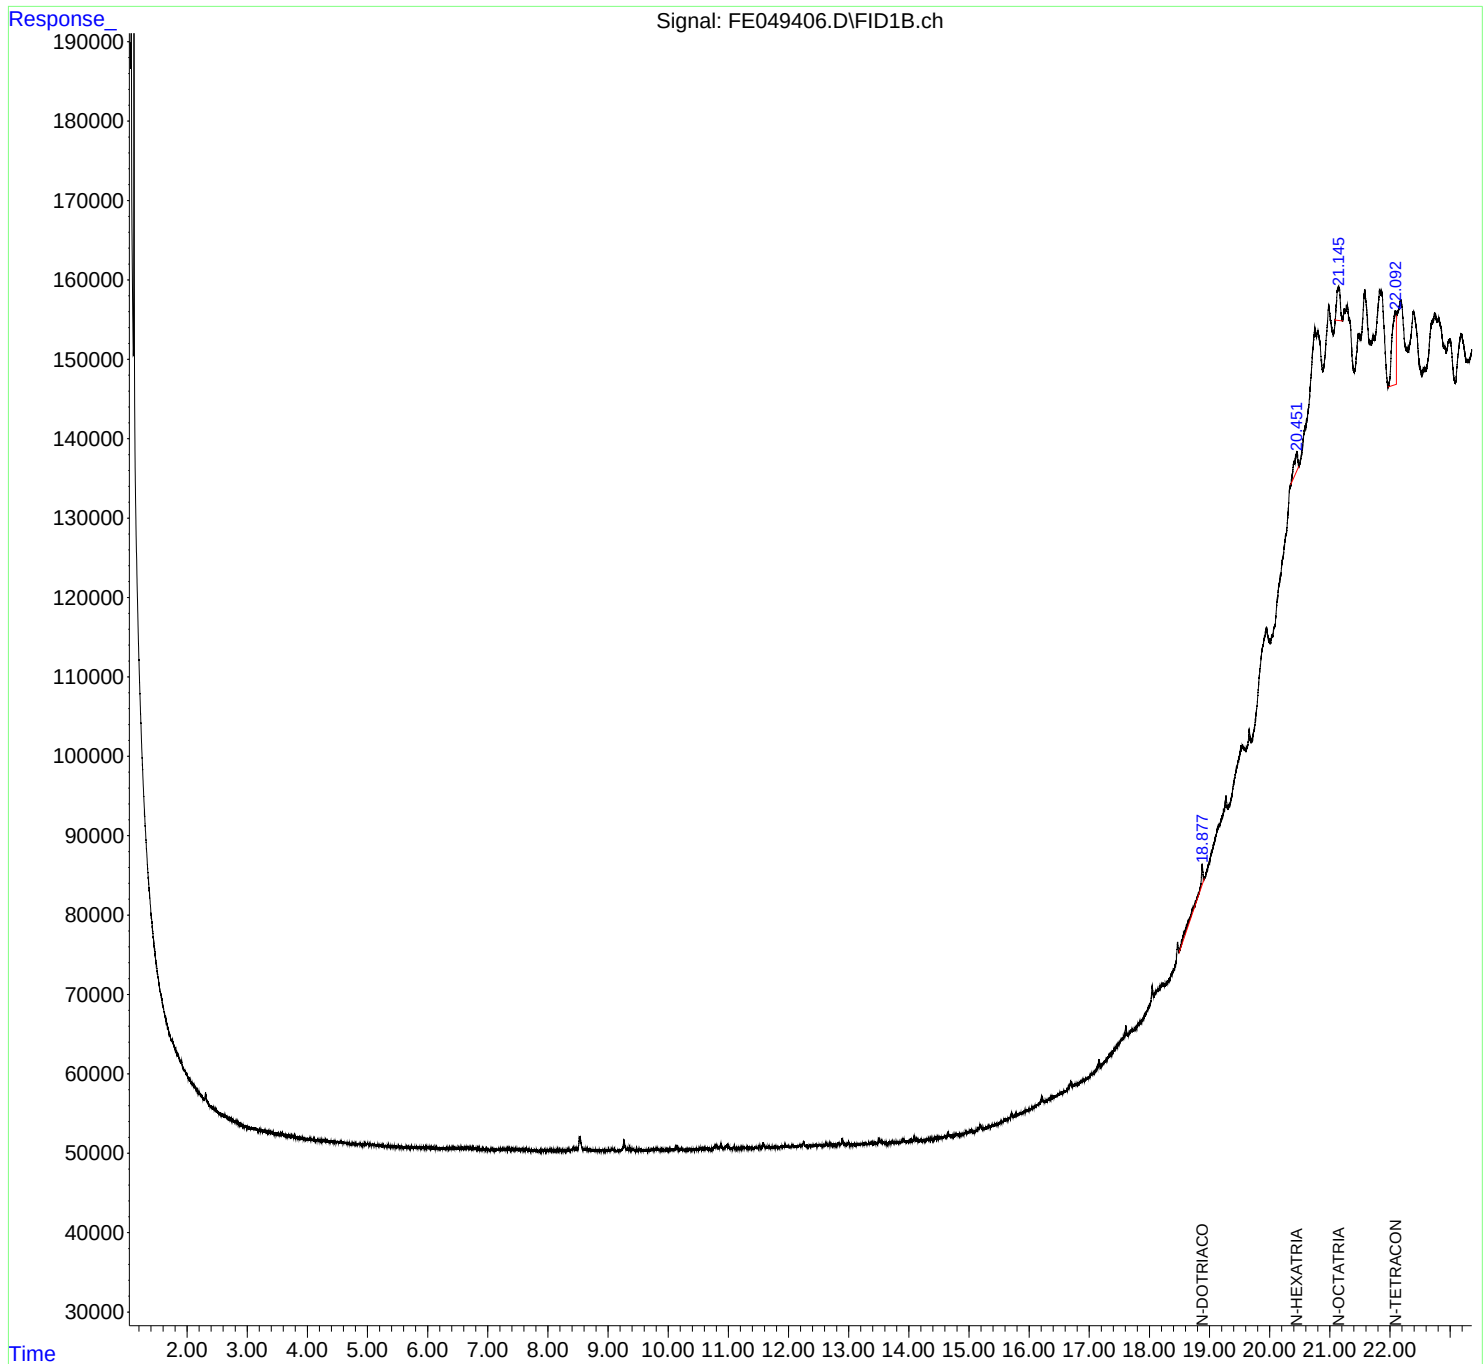


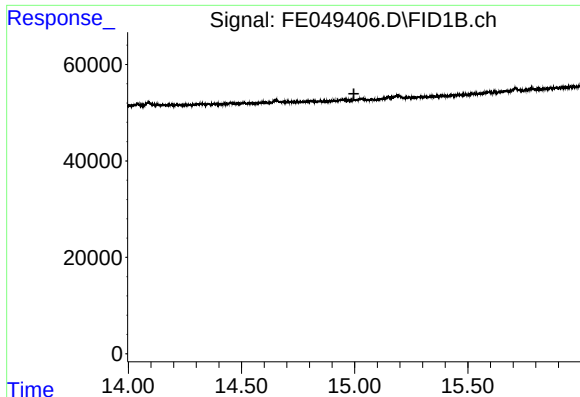

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.996 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

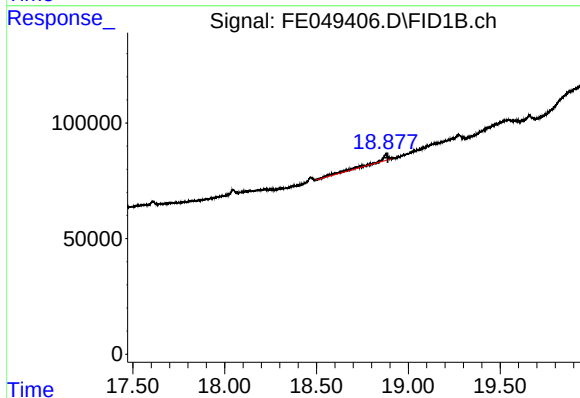


#14 N-DOTRIACONTANE

R.T.: 18.877 min
Delta R.T.: -0.011 min
Response: 107751
Conc: 0.77 ug/ml

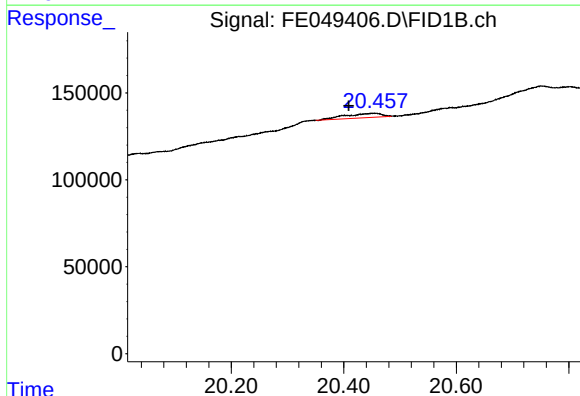


#16 N-HEXATRIACONTANE

R.T.: 20.454 min
Delta R.T.: 0.045 min
Response: 109792
Conc: 1.07 ug/ml

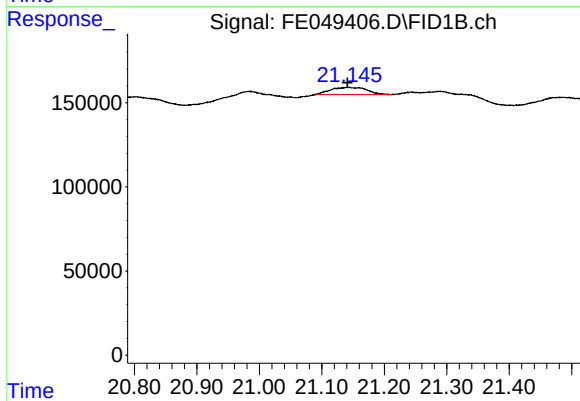

#17 N-OCTATRIACONTANE

R.T.: 21.144 min
Delta R.T.: 0.003 min
Response: 171261
Conc: 1.82 ug/ml

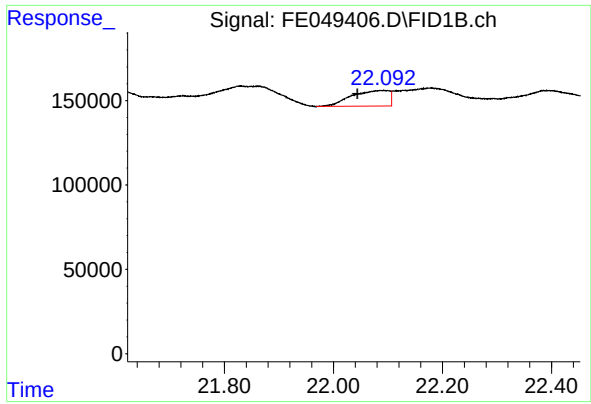

#18 N-TETRACONTANE

R.T.: 22.092 min
Delta R.T.: 0.048 min
Response: 446073
Conc: 4.71 ug/ml

Instrument :
FID_E
ClientSampleId :