

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080224\
Data File : FE049410.D
Signal(s) : FID1B.ch
Acq On : 02 Aug 2024 23:24
Operator : YP\AJ
Sample : PB162367BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 03 03:22:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072924.M
Quant Title :
QLast Update : Tue Jul 30 04:50:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.986	2133517	16.684 ug/ml
Target Compounds			
16) N-HEXATRIACONTANE	20.401	26015	0.254 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080224\
Data File : FE049410.D
Signal(s) : FID1B.ch
Acq On : 02 Aug 2024 23:24
Operator : YP\AJ
Sample : PB162367BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 03 03:22:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072924.M
Quant Title :
QLast Update : Tue Jul 30 04:50:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

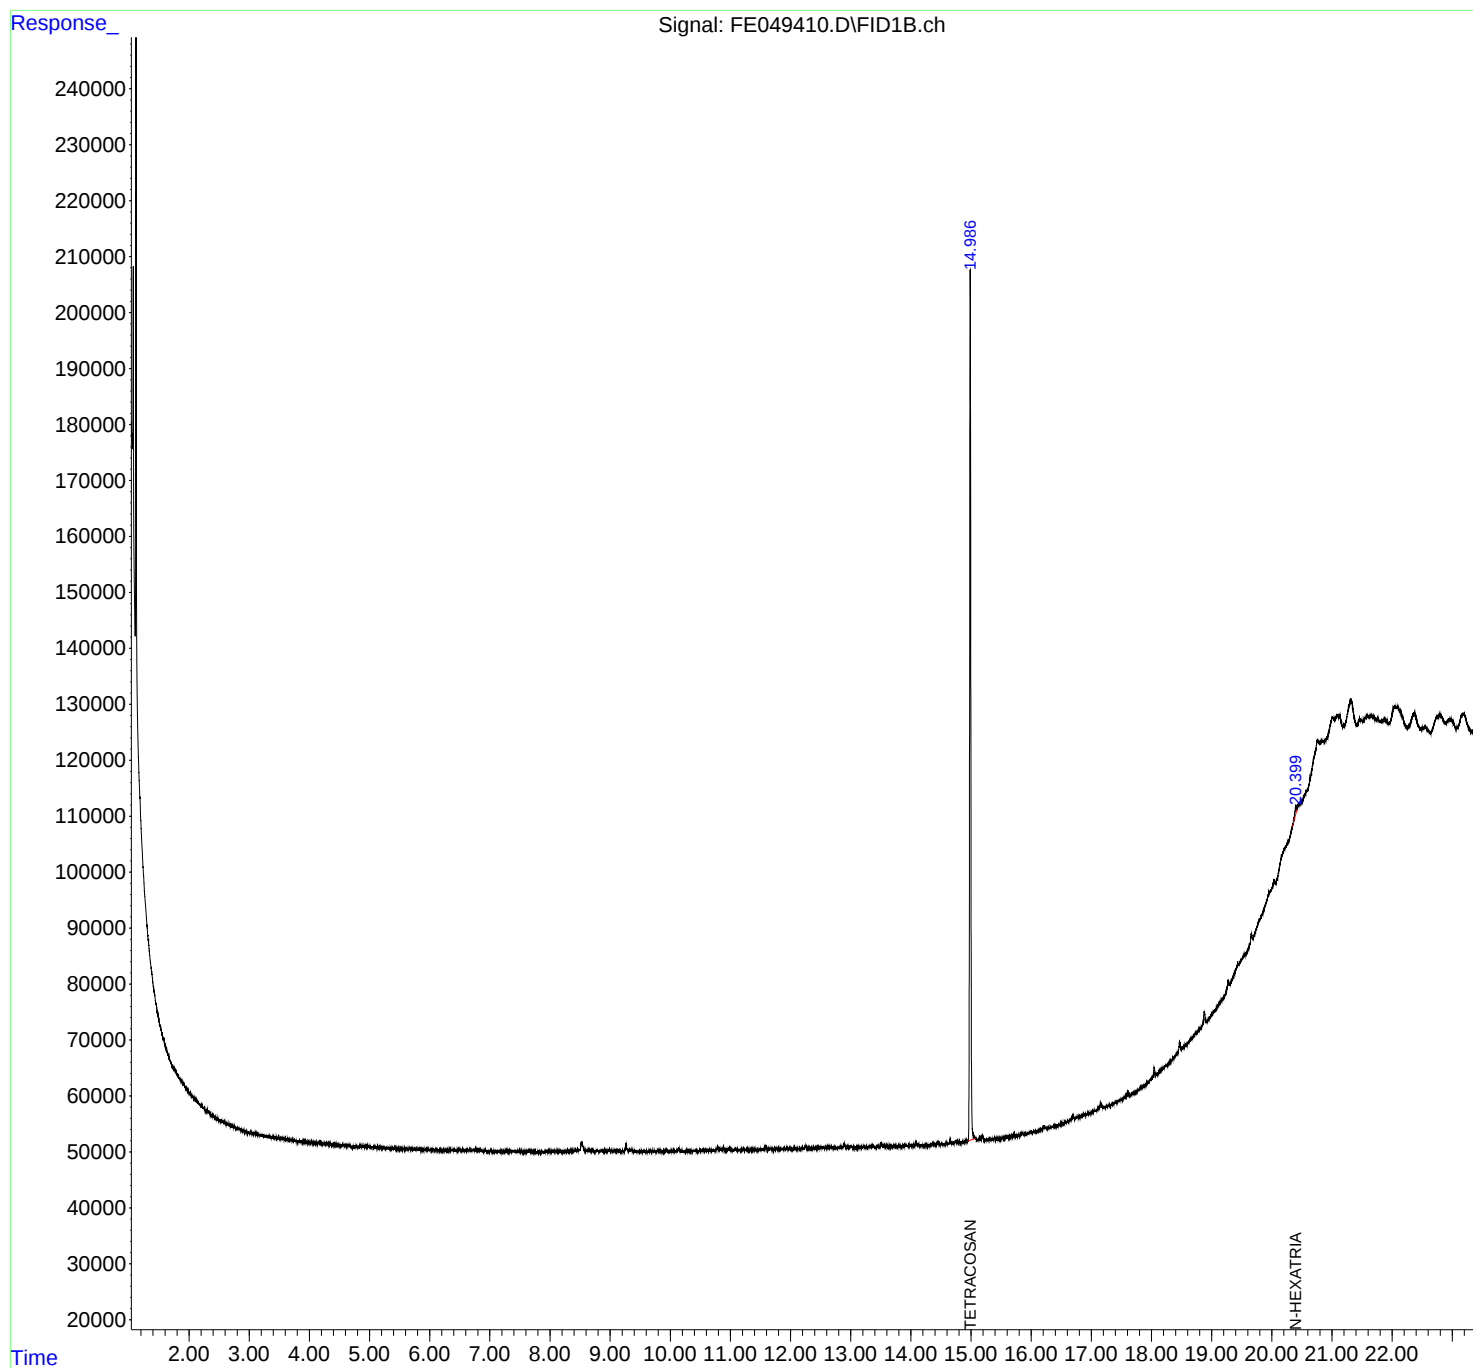


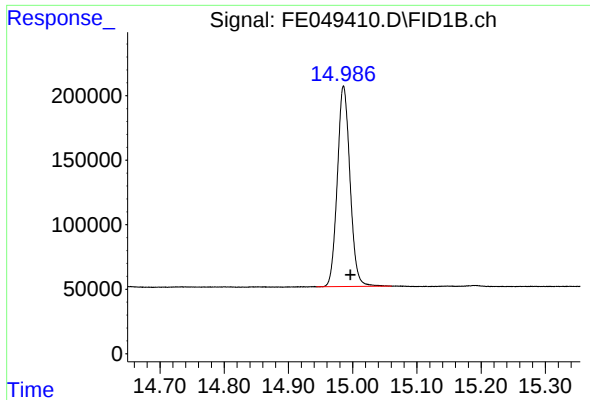

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.986 min
Delta R.T.: -0.010 min
Response: 2133517
Conc: 16.68 ug/ml

Instrument :
FID_E
ClientSampleId :

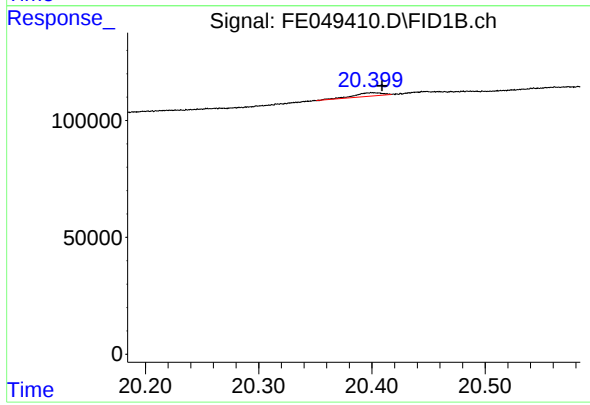

#16 N-HEXATRIACONTANE

R.T.: 20.401 min
Delta R.T.: -0.008 min
Response: 26015
Conc: 0.25 ug/ml