

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
Data File : FE032492.D
Signal(s) : FID1B.CH
Acq On : 03 Aug 2020 9:54
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Aug 04 00:45:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
Quant Title :
QLast Update : Wed Jul 29 02:31:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
16) N-HEXATRIACONTANE	20.166	31391	0.143 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
Data File : FE032492.D
Signal(s) : FID1B.CH
Acq On : 03 Aug 2020 9:54
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Aug 04 00:45:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
Quant Title :
QLast Update : Wed Jul 29 02:31:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

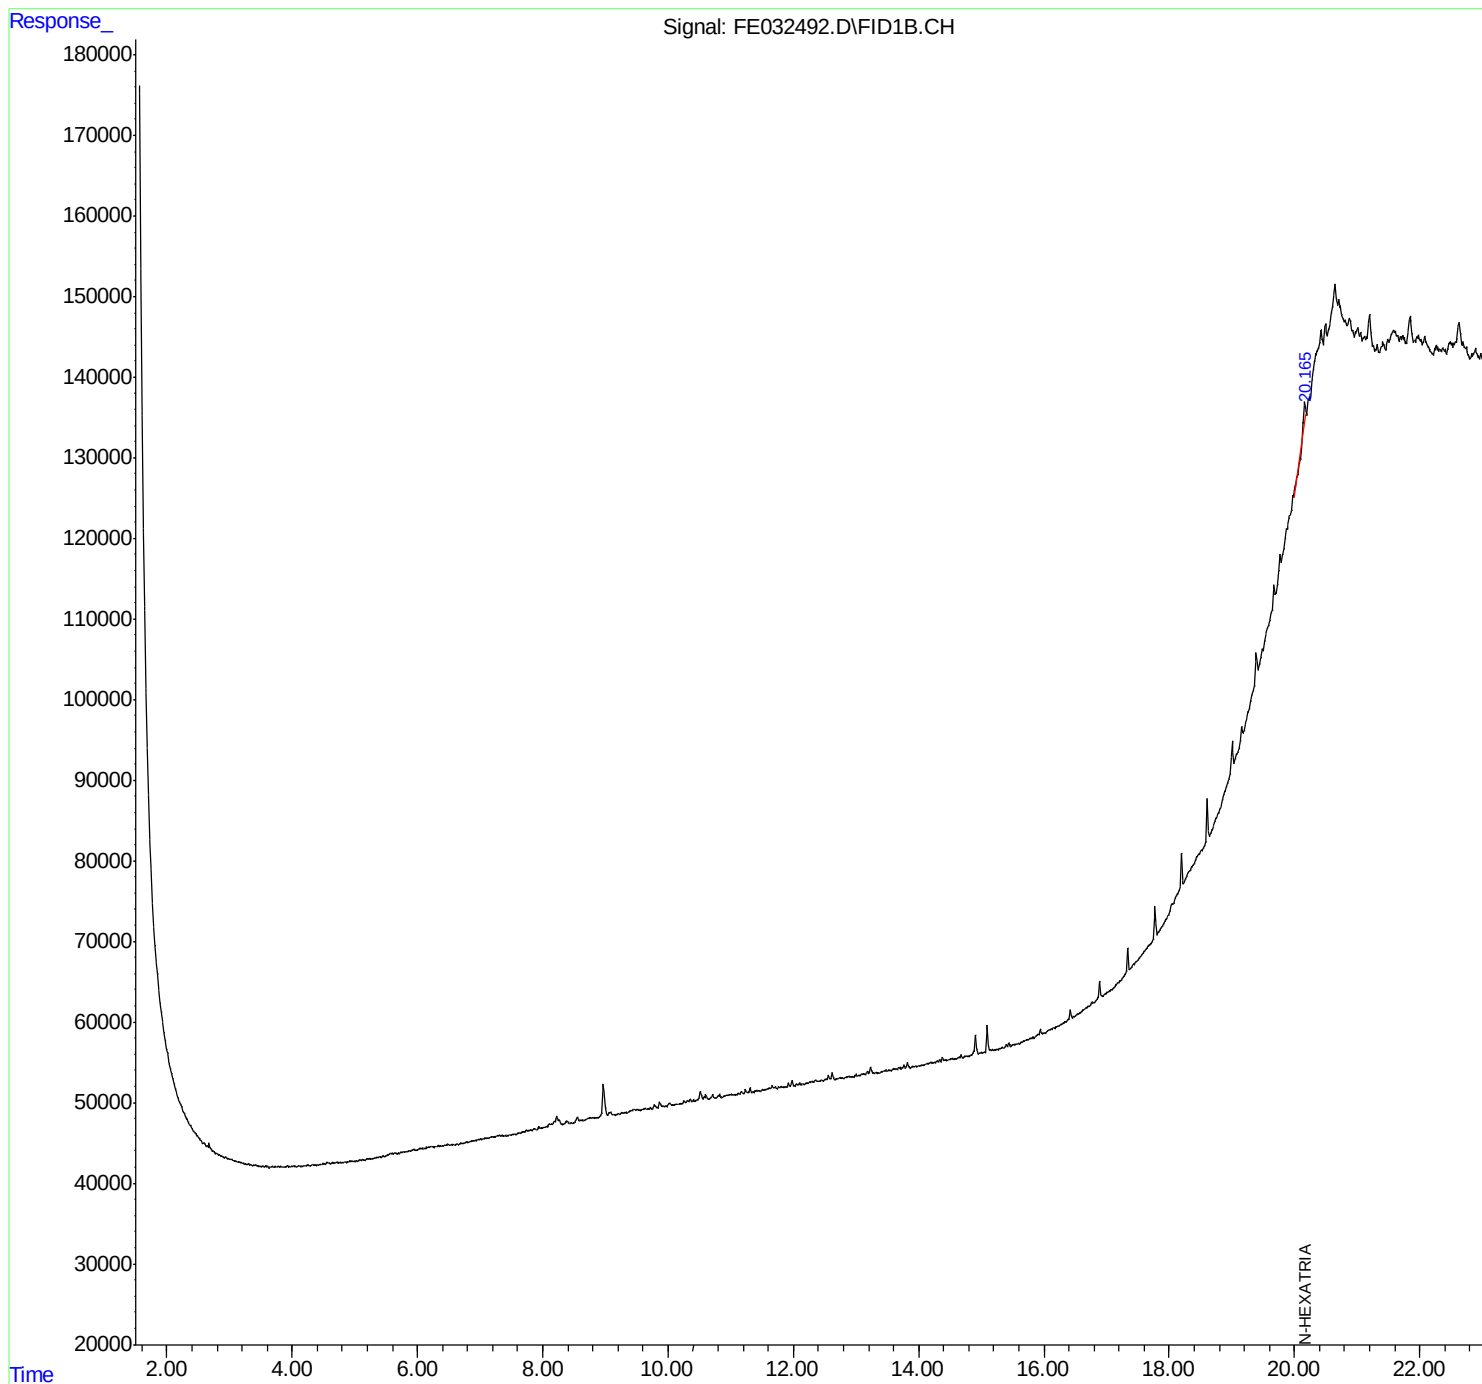


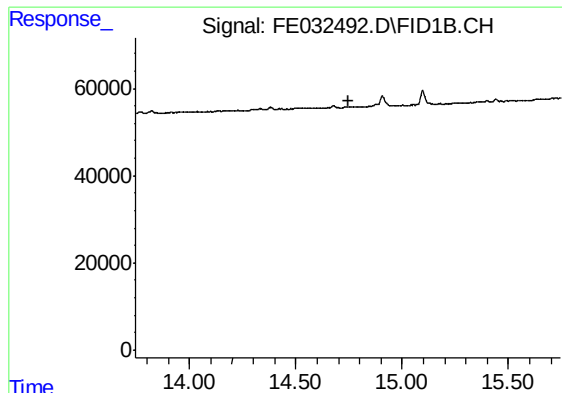

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.745 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
MECL2

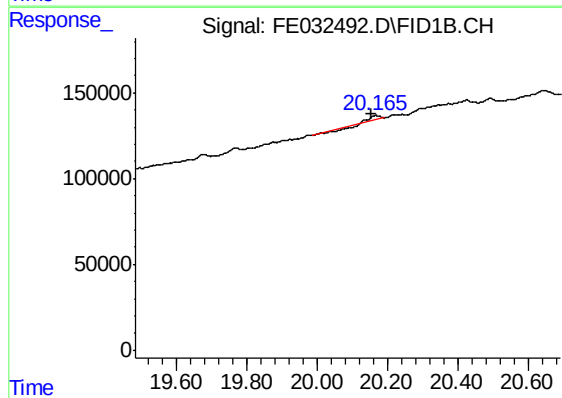

#16 N-HEXATRIACONTANE

R.T.: 20.166 min
Delta R.T.: 0.012 min
Response: 31391
Conc: 0.14 ug/ml