

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
 Data File : FE032497.D
 Signal(s) : FID1B.CH
 Acq On : 03 Aug 2020 14:37
 Operator : DD\AJ
 Sample : L3535-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 JTY1-SB-0203

Integration File: autoint1.e
 Quant Time: Aug 04 00:46:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
 Quant Title :
 QLast Update : Wed Jul 29 02:31:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.719	3609278	11.248 ug/ml
Target Compounds			
4) N-TETRADECANE	8.337	1123646	3.099 ug/ml
7) N-EICOSANE	12.692	106786	0.288 ug/ml
10) N-TETRACOSANE	14.912	125598	0.337 ug/ml
12) N-OCTACOSANE	16.888	178358	0.484 ug/ml
13) N-TRIACONTANE	17.777	250211	0.682 ug/ml
14) N-DOTRIACONTANE	18.602	379465	1.098 ug/ml
15) N-TETRATRIACONTANE	19.431	100101	0.348 ug/ml
16) N-HEXATRIACONTANE	20.164	87649	0.400 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
Data File : FE032497.D
Signal(s) : FID1B.CH
Acq On : 03 Aug 2020 14:37
Operator : DD\AJ
Sample : L3535-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JTY1-SB-0203

Integration File: autoint1.e
Quant Time: Aug 04 00:46:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
Quant Title :
QLast Update : Wed Jul 29 02:31:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

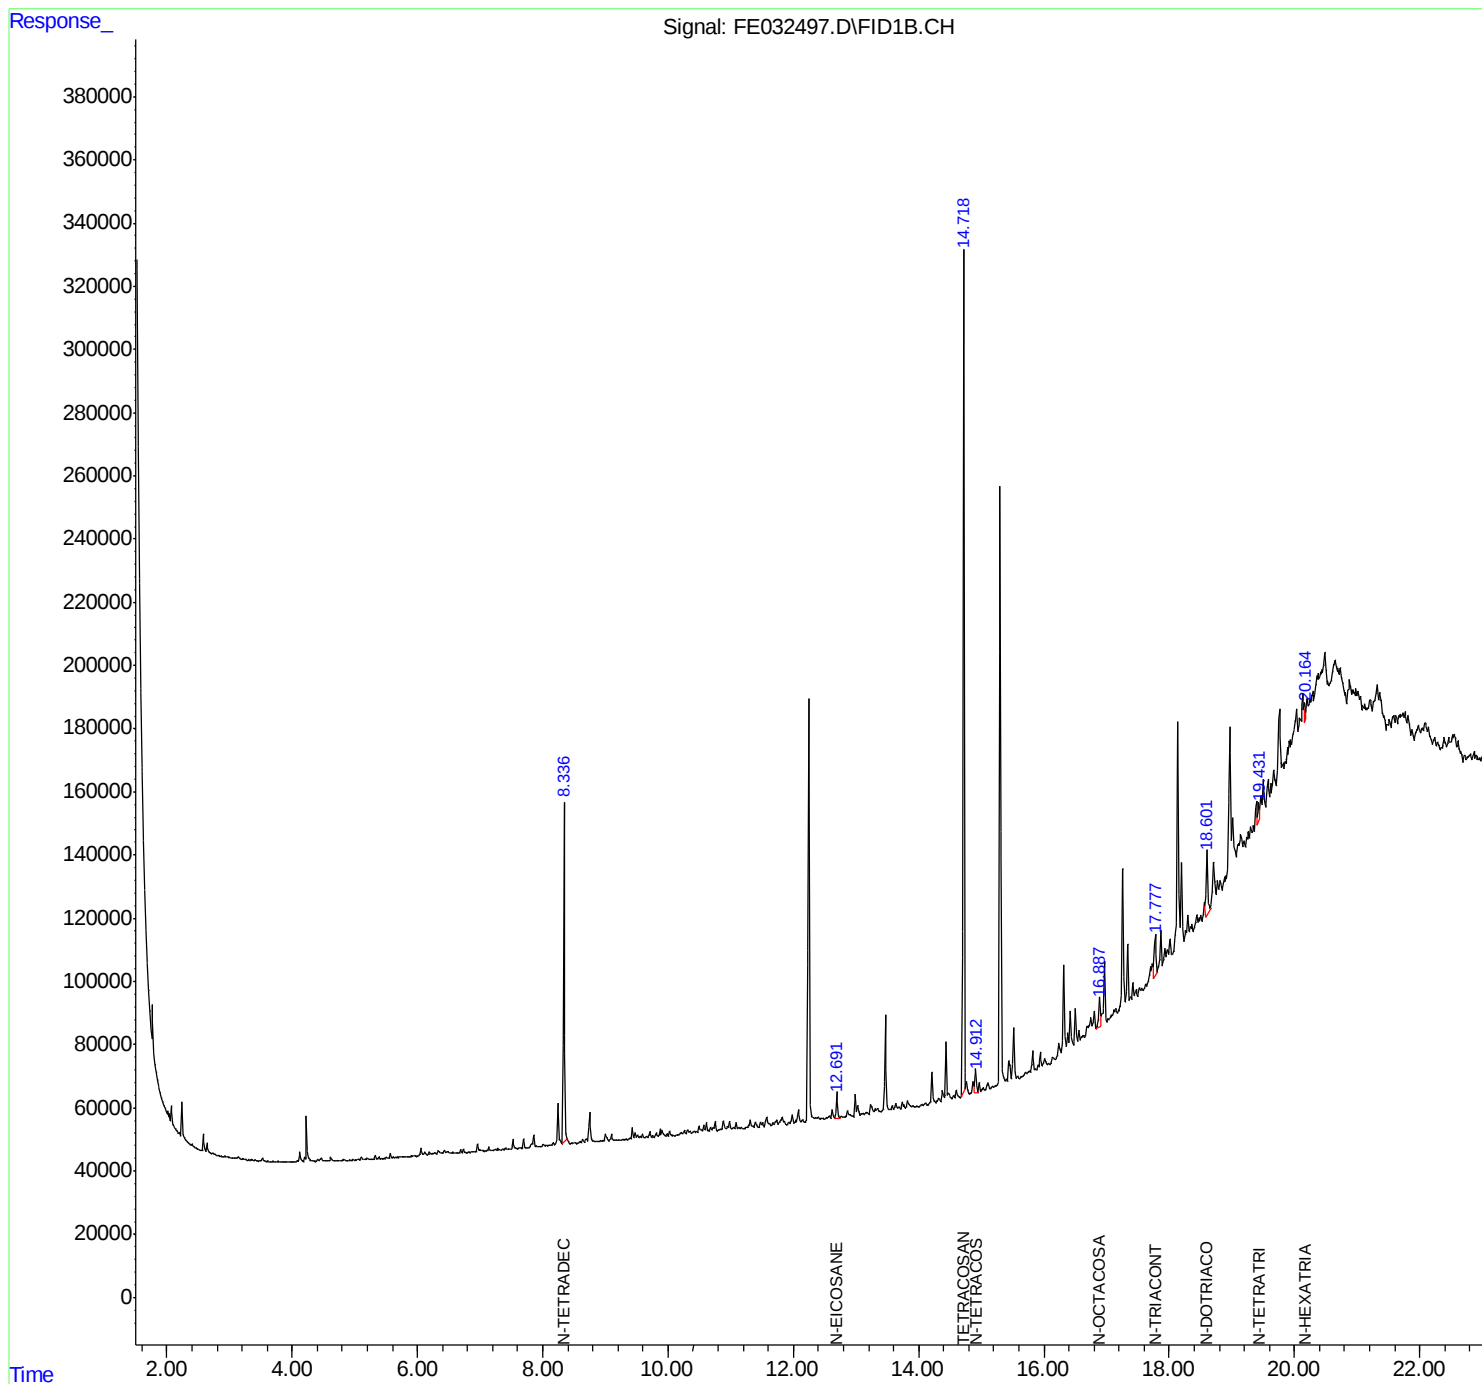


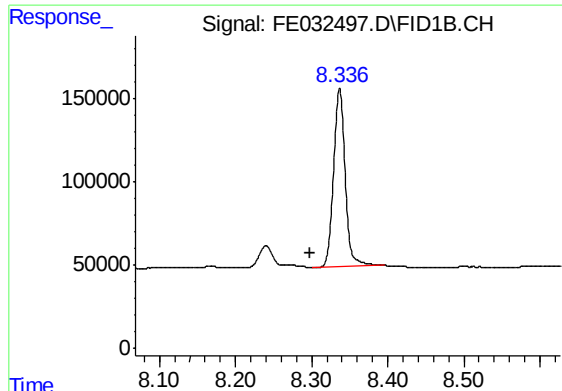

#4 N-TETRADECANE


R.T.: 8.337 min
Delta R.T.: 0.038 min
Response: 1123646
Conc: 3.10 ug/ml

Instrument :
FID_E
ClientSampleId :
JTY1-SB-0203

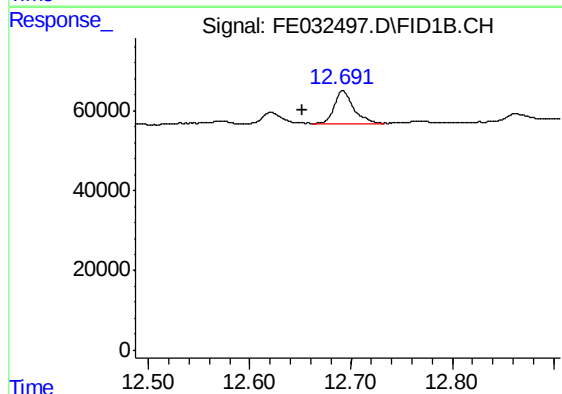


#7 N-EICOSANE

R.T.: 12.692 min
Delta R.T.: 0.040 min
Response: 106786
Conc: 0.29 ug/ml

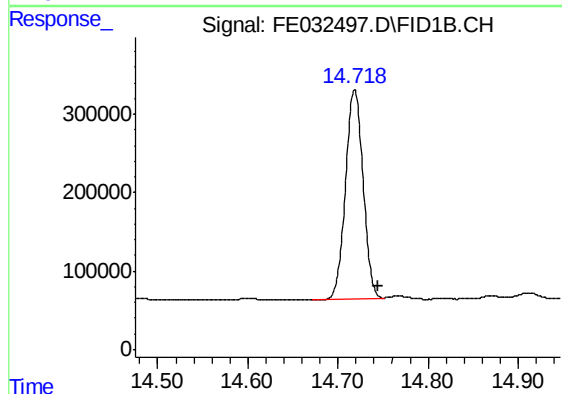


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.719 min
Delta R.T.: -0.026 min
Response: 3609278
Conc: 11.25 ug/ml

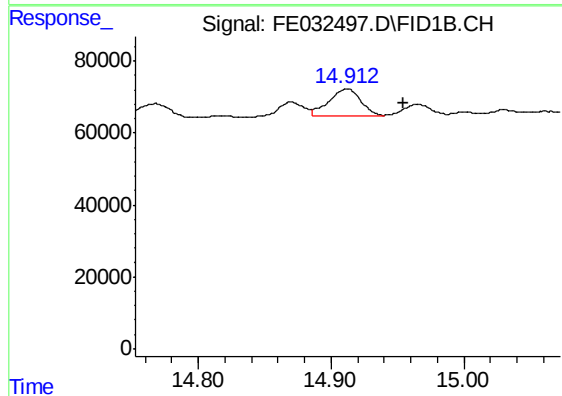

#10 N-TETRACOSANE


R.T.: 14.912 min
Delta R.T.: -0.042 min
Response: 125598
Conc: 0.34 ug/ml

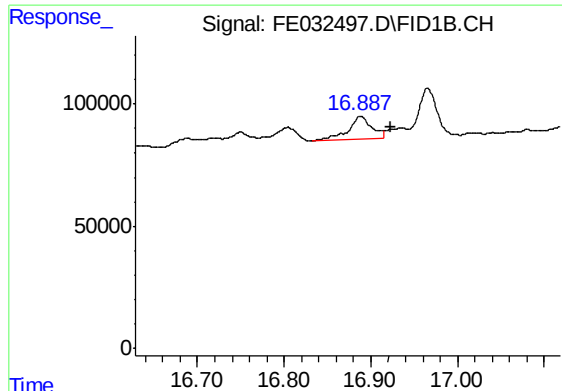

#12 N-OCTACOSANE


R.T.: 16.888 min
Delta R.T.: -0.035 min
Response: 178358
Conc: 0.48 ug/ml

Instrument :
FID_E
ClientSampleId :
JTY1-SB-0203

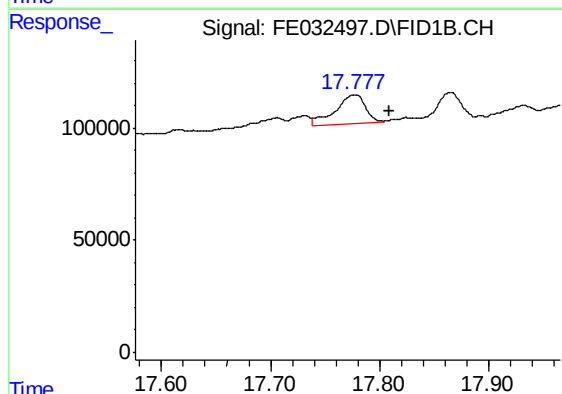


#13 N-TRIACONTANE

R.T.: 17.777 min
Delta R.T.: -0.032 min
Response: 250211
Conc: 0.68 ug/ml

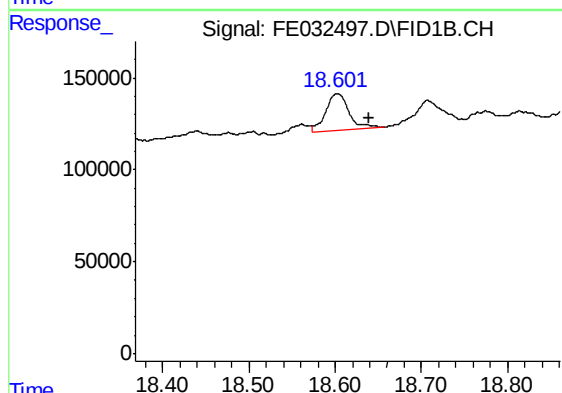


#14 N-DOTRIACONTANE

R.T.: 18.602 min
Delta R.T.: -0.038 min
Response: 379465
Conc: 1.10 ug/ml

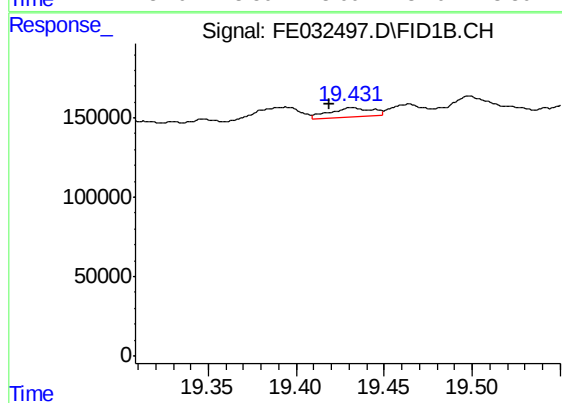

#15 N-TETRATRIACONTANE

R.T.: 19.431 min
Delta R.T.: 0.012 min
Response: 100101
Conc: 0.35 ug/ml

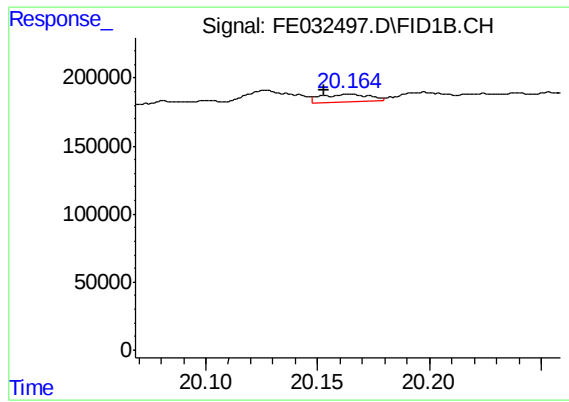

#16 N-HEXATRIACONTANE

R.T.: 20.164 min
Delta R.T.: 0.011 min
Response: 87649
Conc: 0.40 ug/ml

Instrument :
FID_E
ClientSampleId :
JTY1-SB-0203