

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
 Data File : FE032499.D
 Signal(s) : FID1B.CH
 Acq On : 03 Aug 2020 15:45
 Operator : DD\AJ
 Sample : L3535-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 JTY1-SB-101

Integration File: autoint1.e
 Quant Time: Aug 04 00:46:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
 Quant Title :
 QLast Update : Wed Jul 29 02:31:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.721	6469200	20.160 ug/ml
Target Compounds			
4) N-TETRADECANE	8.338	2106343	5.809 ug/ml
7) N-EICOSANE	12.692	424606	1.147 ug/ml
10) N-TETRACOSANE	14.909	238959	0.641 ug/ml
12) N-OCTACOSANE	16.886	230268	0.625 ug/ml
13) N-TRIACONTANE	17.774	209652	0.571 ug/ml
14) N-DOTRIACONTANE	18.598	352973	1.021 ug/ml
15) N-TETRATRIACONTANE	19.386	133859	0.465 ug/ml
16) N-HEXATRIACONTANE	20.126	180078	0.821 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
Data File : FE032499.D
Signal(s) : FID1B.CH
Acq On : 03 Aug 2020 15:45
Operator : DD\AJ
Sample : L3535-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JTY1-SB-101

Integration File: autoint1.e
Quant Time: Aug 04 00:46:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
Quant Title :
QLast Update : Wed Jul 29 02:31:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

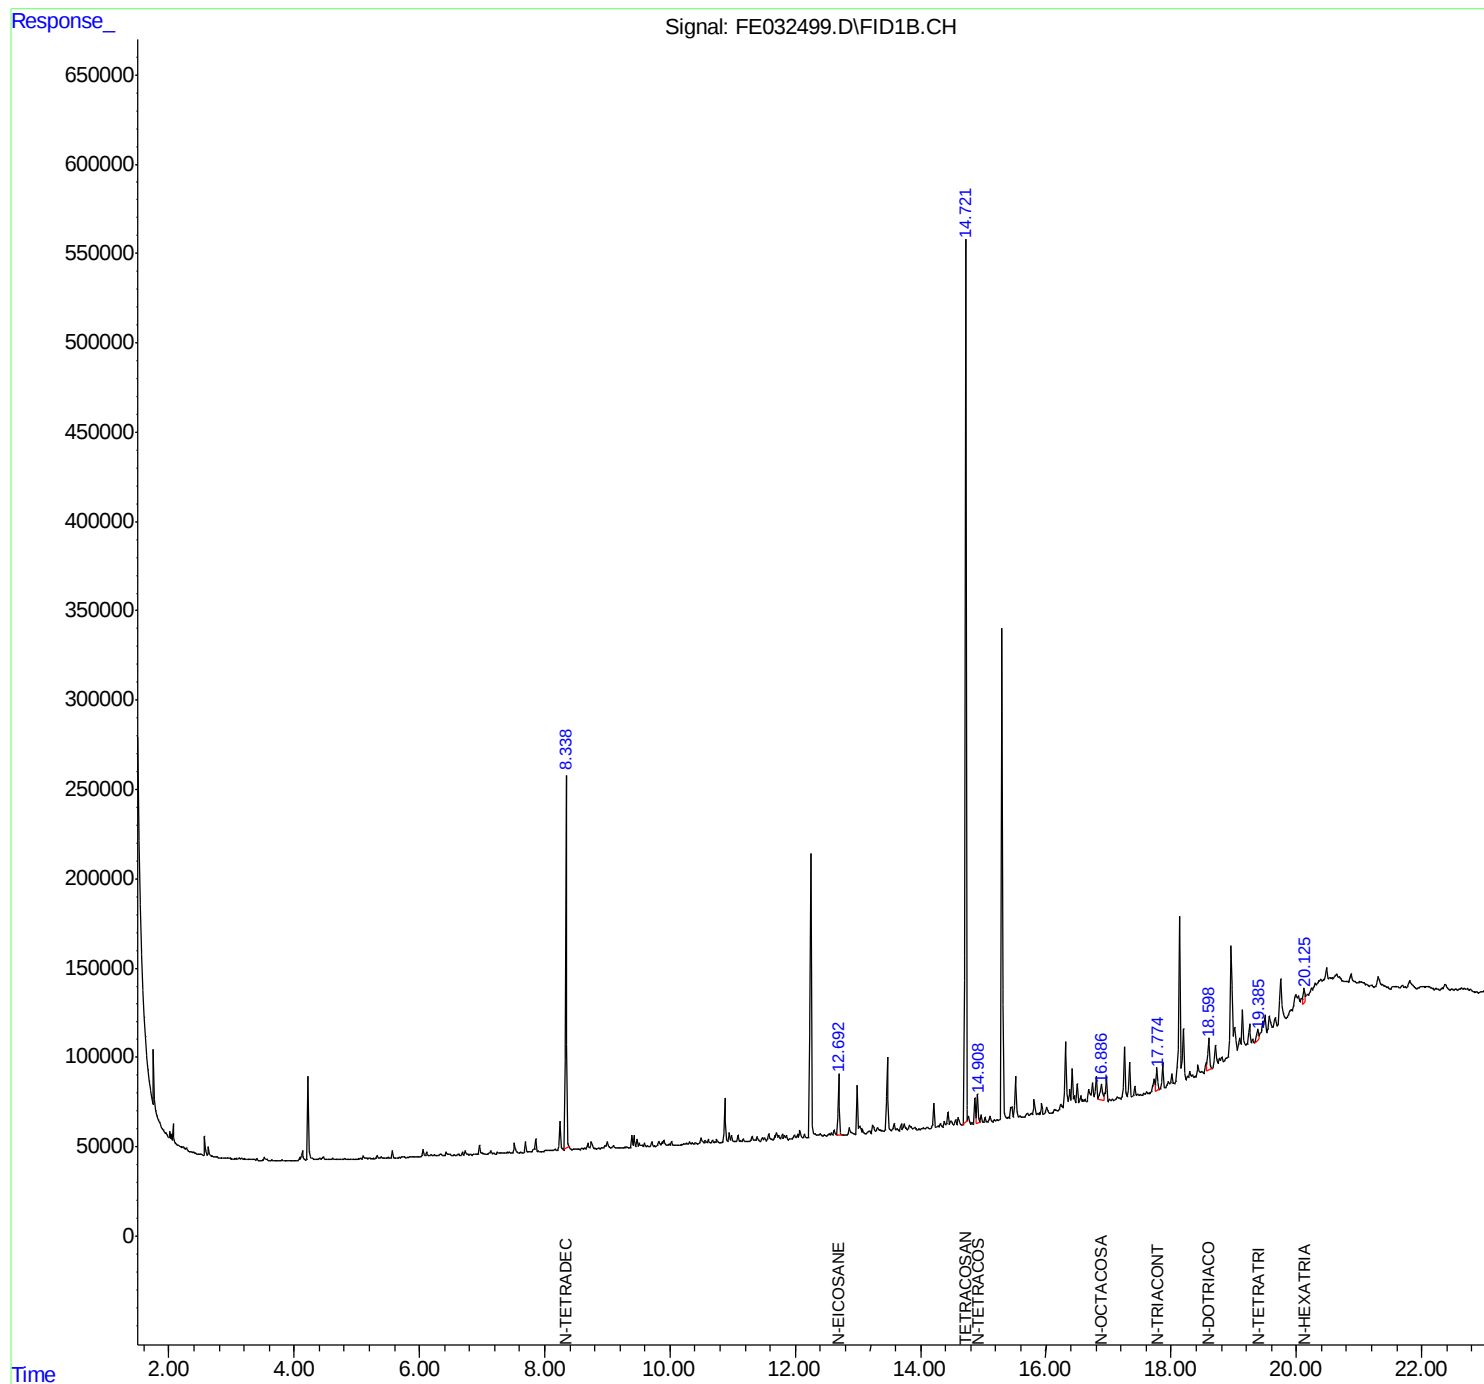


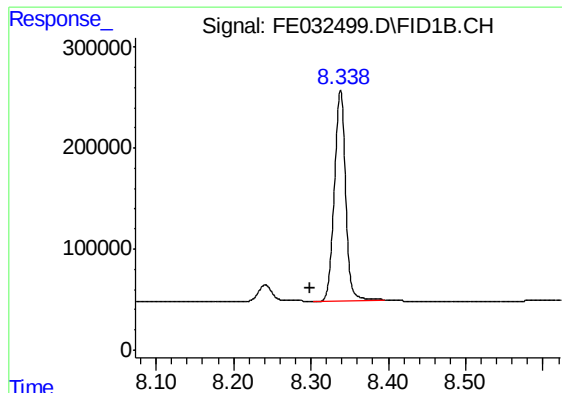

#4 N-TETRADECANE


R.T.: 8.338 min
Delta R.T.: 0.040 min
Response: 2106343
Conc: 5.81 ug/ml

Instrument :
FID_E
ClientSampleId :
JTY1-SB-101

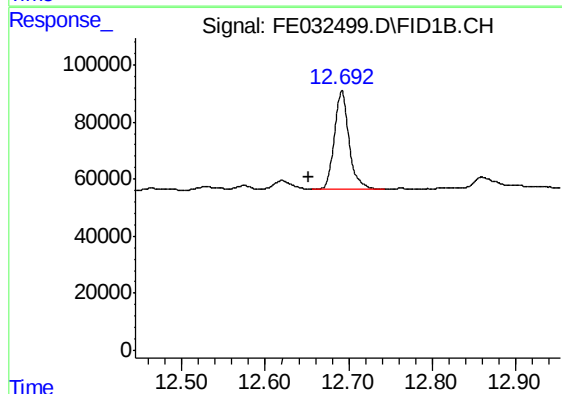


#7 N-EICOSANE

R.T.: 12.692 min
Delta R.T.: 0.040 min
Response: 424606
Conc: 1.15 ug/ml

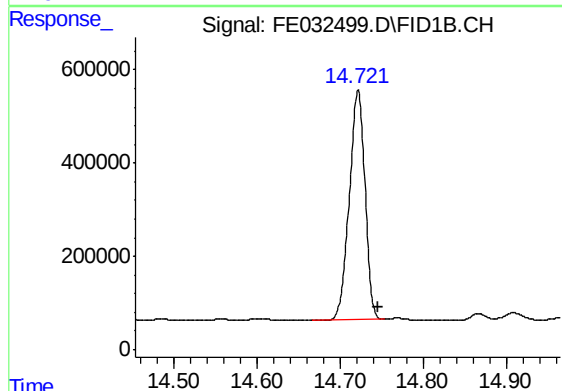


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.721 min
Delta R.T.: -0.024 min
Response: 6469200
Conc: 20.16 ug/ml

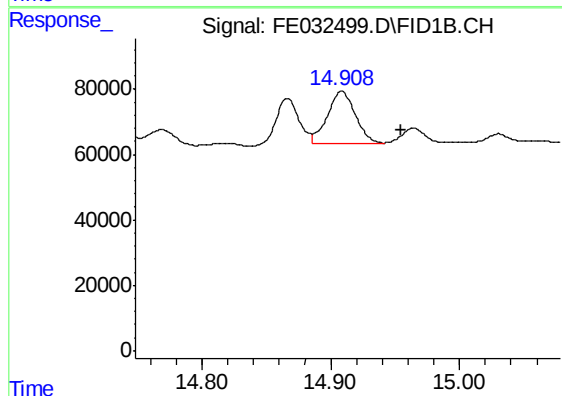

#10 N-TETRACOSANE


R.T.: 14.909 min
Delta R.T.: -0.046 min
Response: 238959
Conc: 0.64 ug/ml

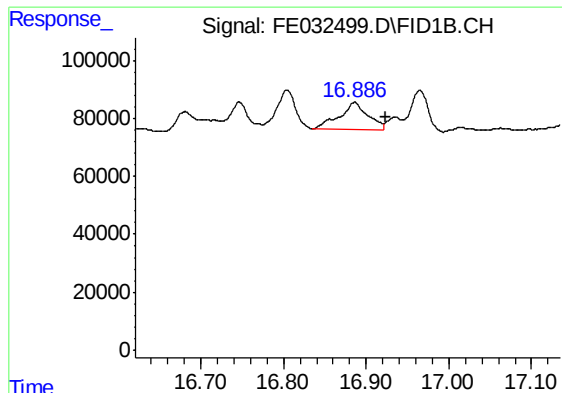

#12 N-OCTACOSANE


R.T.: 16.886 min
Delta R.T.: -0.037 min
Response: 230268
Conc: 0.63 ug/ml

Instrument :
FID_E
ClientSampleId :
JTY1-SB-101

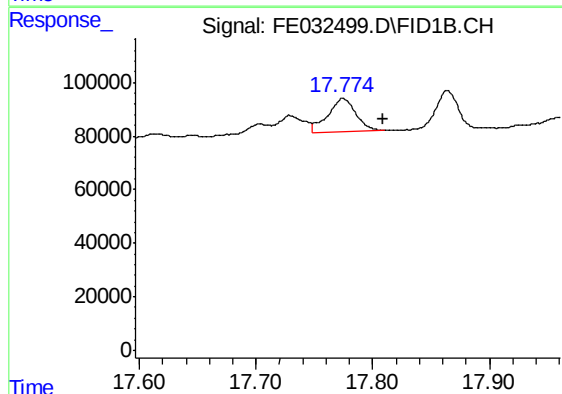


#13 N-TRIACONTANE

R.T.: 17.774 min
Delta R.T.: -0.035 min
Response: 209652
Conc: 0.57 ug/ml

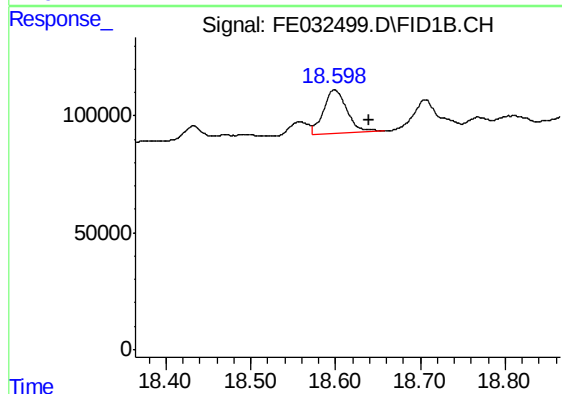


#14 N-DOTRIACONTANE

R.T.: 18.598 min
Delta R.T.: -0.041 min
Response: 352973
Conc: 1.02 ug/ml

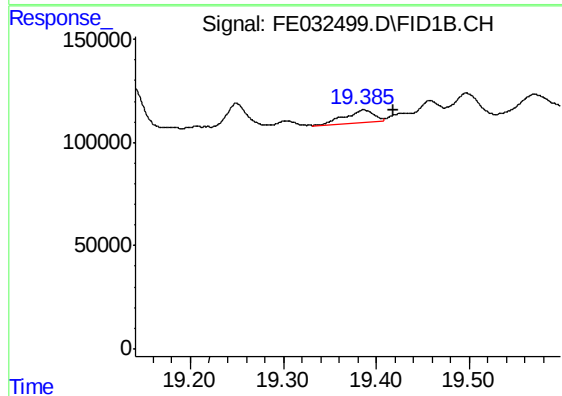

#15 N-TETRATRIACONTANE

R.T.: 19.386 min
Delta R.T.: -0.032 min
Response: 133859
Conc: 0.47 ug/ml

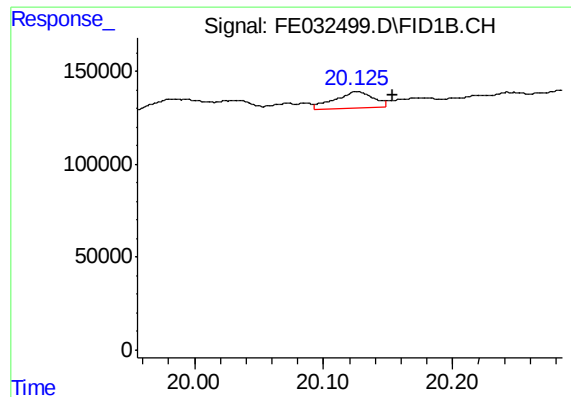

#16 N-HEXATRIACONTANE

R.T.: 20.126 min
Delta R.T.: -0.027 min
Response: 180078
Conc: 0.82 ug/ml

Instrument :
FID_E
ClientSampleId :
JTY1-SB-101