

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
 Data File : FE032501.D
 Signal(s) : FID1B.CH
 Acq On : 03 Aug 2020 16:54
 Operator : DD\AJ
 Sample : L3537-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 JTY1-WC-S-0203

Integration File: autoint1.e
 Quant Time: Aug 04 00:47:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
 Quant Title :
 QLast Update : Wed Jul 29 02:31:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.767	117868	0.367 ug/ml
Target Compounds			
4) N-TETRADECANE	8.340	2654037	7.319 ug/ml
7) N-EICOSANE	12.691	199241	0.538 ug/ml
10) N-TETRACOSANE	14.965	69525	0.186 ug/ml
11) N-HEXACOSANE	15.941	131584	0.357 ug/ml
12) N-OCTACOSANE	16.889	357657	0.971 ug/ml
13) N-TRIACONTANE	17.777	554478	1.511 ug/ml
14) N-DOTRIACONTANE	18.603	1040993	3.012 ug/ml
15) N-TETRATRIACONTANE	19.436	177805	0.618 ug/ml
16) N-HEXATRIACONTANE	20.136	397614	1.813 ug/ml
17) N-OCTATRIACONTANE	20.882	153660	0.876 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
Data File : FE032501.D
Signal(s) : FID1B.CH
Acq On : 03 Aug 2020 16:54
Operator : DD\AJ
Sample : L3537-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JTY1-WC-S-0203

Integration File: autoint1.e
Quant Time: Aug 04 00:47:05 2020
Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
Quant Title :
QLast Update : Wed Jul 29 02:31:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

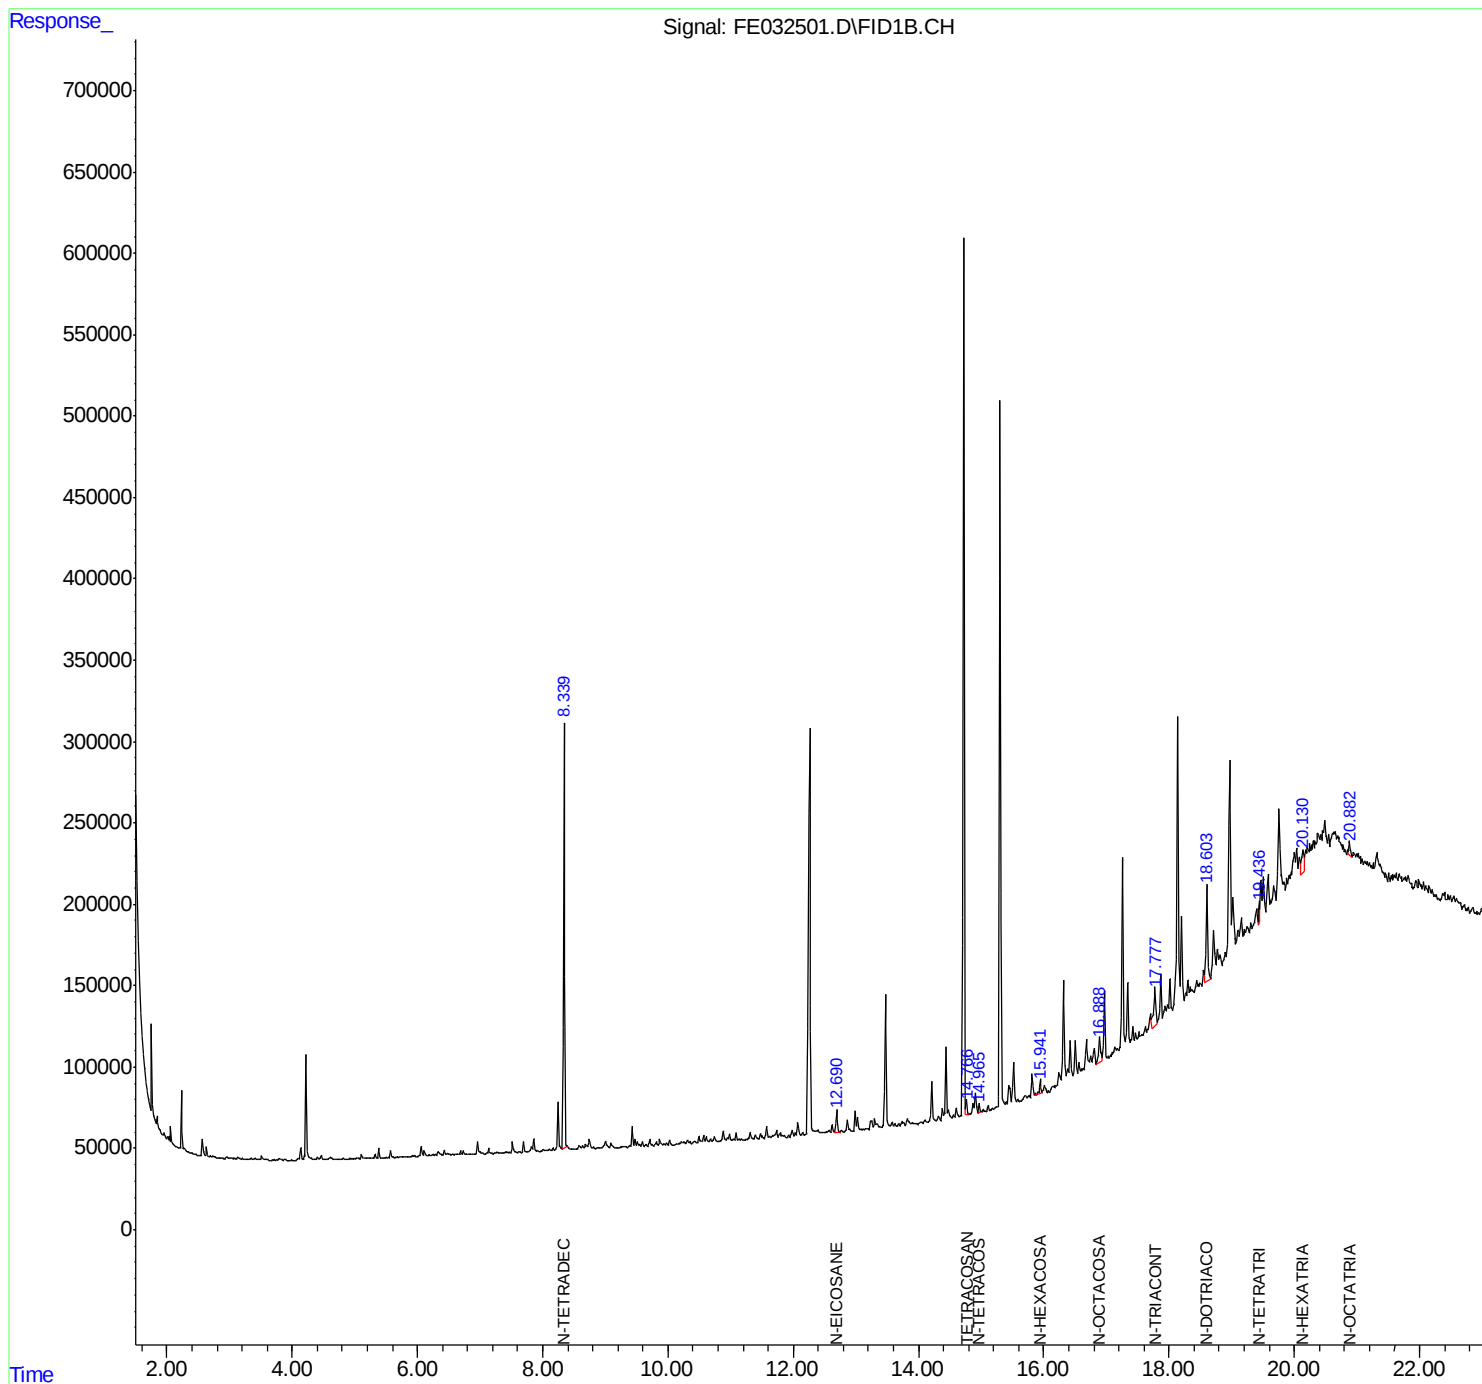


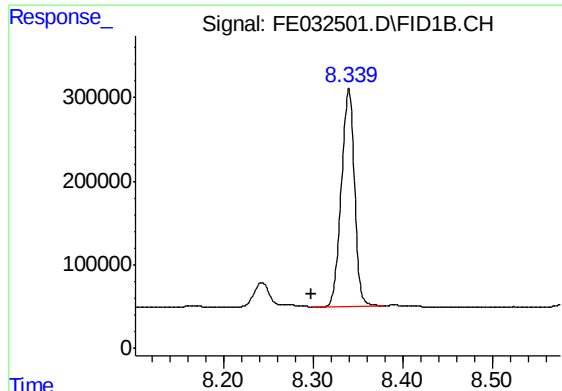

#4 N-TETRADECANE


R.T.: 8.340 min
Delta R.T.: 0.041 min
Response: 2654037
Conc: 7.32 ug/ml

Instrument :
FID_E
ClientSampleId :
JTY1-WC-S-0203

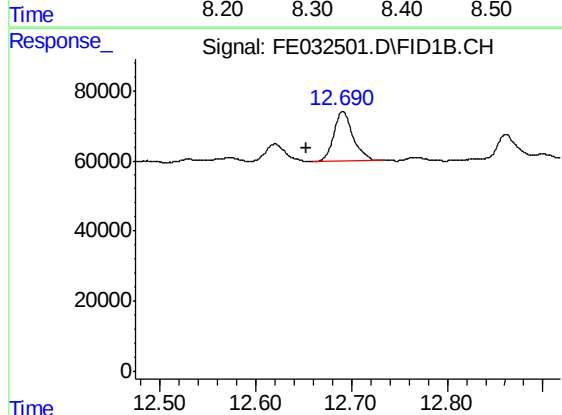


#7 N-EICOSANE

R.T.: 12.691 min
Delta R.T.: 0.039 min
Response: 199241
Conc: 0.54 ug/ml

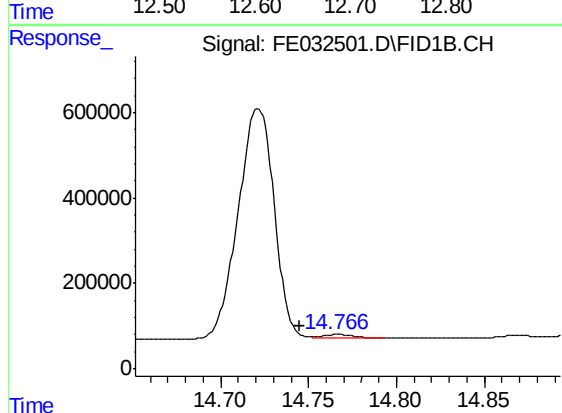


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.767 min
Delta R.T.: 0.022 min
Response: 117868
Conc: 0.37 ug/ml

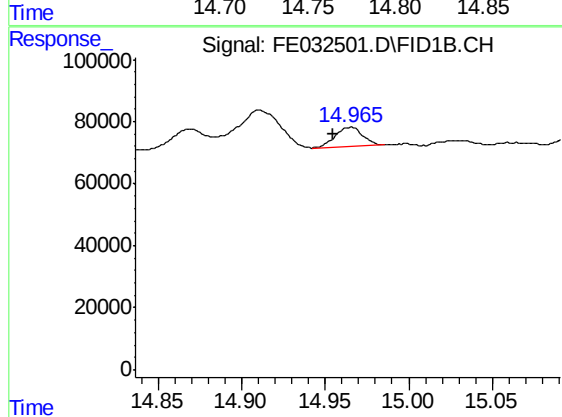

#10 N-TETRACOSANE


R.T.: 14.965 min
Delta R.T.: 0.011 min
Response: 69525
Conc: 0.19 ug/ml

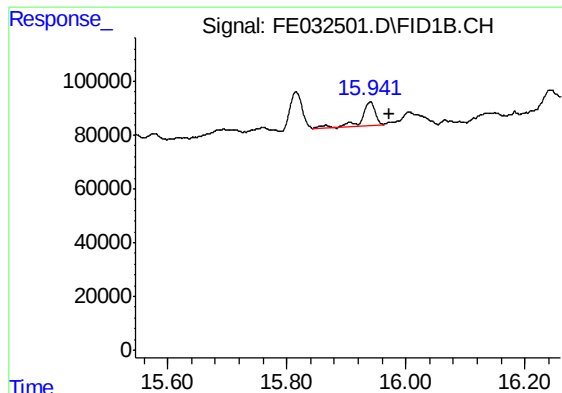

#11 N-HEXACOSANE


R.T.: 15.941 min
Delta R.T.: -0.033 min
Response: 131584
Conc: 0.36 ug/ml

Instrument :
FID_E
ClientSampleId :
JTY1-WC-S-0203

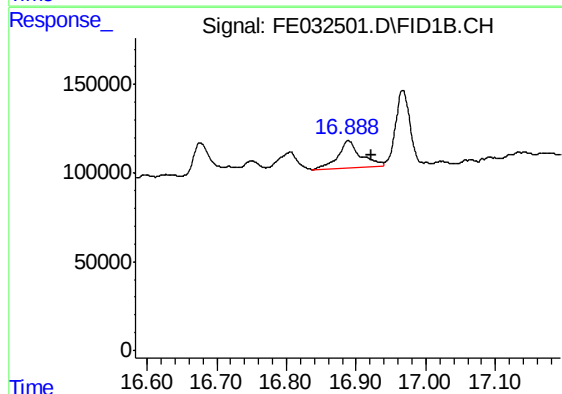


#12 N-OCTACOSANE

R.T.: 16.889 min
Delta R.T.: -0.034 min
Response: 357657
Conc: 0.97 ug/ml

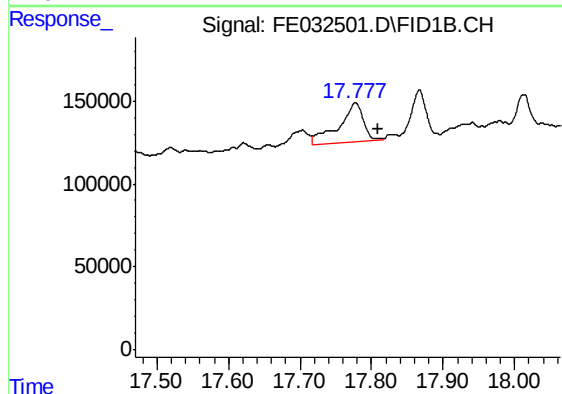


#13 N-TRIACONTANE

R.T.: 17.777 min
Delta R.T.: -0.032 min
Response: 554478
Conc: 1.51 ug/ml

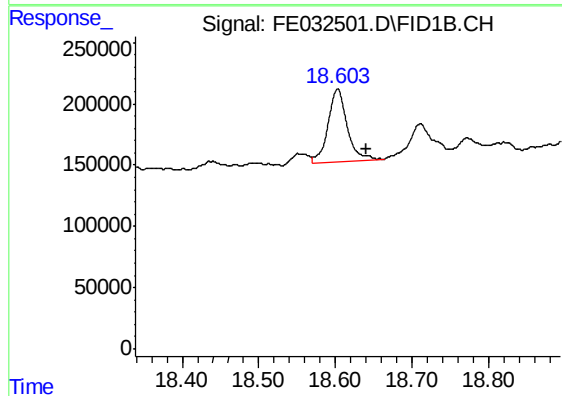

#14 N-DOTRIACONTANE


R.T.: 18.603 min
Delta R.T.: -0.036 min
Response: 1040993
Conc: 3.01 ug/ml

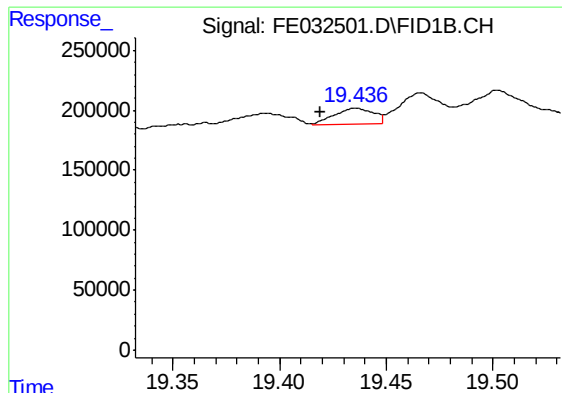

#15 N-TETRATRIACONTANE


R.T.: 19.436 min
Delta R.T.: 0.017 min
Response: 177805
Conc: 0.62 ug/ml

Instrument :
FID_E
ClientSampleId :
JTY1-WC-S-0203

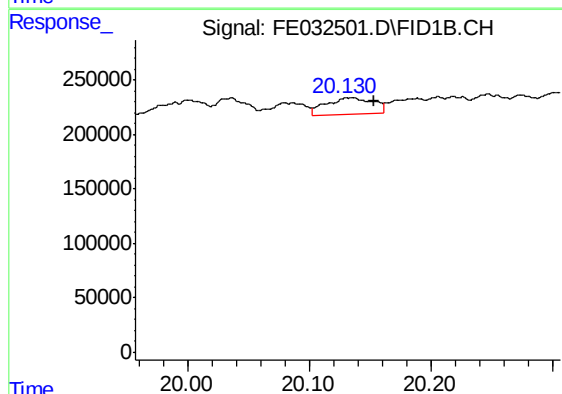

#16 N-HEXATRIACONTANE

R.T.: 20.136 min
Delta R.T.: -0.017 min
Response: 397614
Conc: 1.81 ug/ml

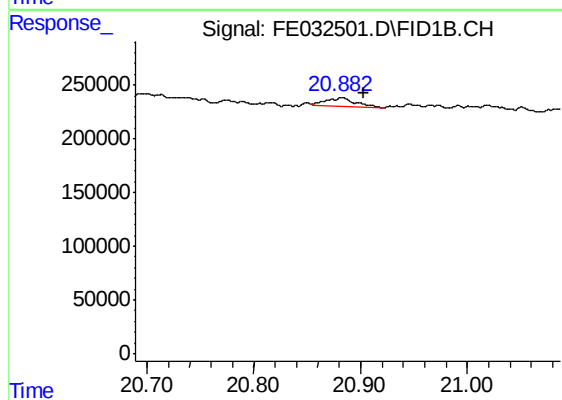

#17 N-OCTATRIACONTANE

R.T.: 20.882 min
Delta R.T.: -0.020 min
Response: 153660
Conc: 0.88 ug/ml