

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
 Data File : FE032507.D
 Signal(s) : FID1B.CH
 Acq On : 03 Aug 2020 20:19
 Operator : DD\AJ
 Sample : PB130684BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 PB130684BL

Integration File: autoint1.e
 Quant Time: Aug 04 00:48:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
 Quant Title :
 QLast Update : Wed Jul 29 02:31:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.717	5436061	16.941 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.773	175225	0.477 ug/ml
14) N-DOTRIACONTANE	18.603	208141	0.602 ug/ml
15) N-TETRATRIACONTANE	19.384	145949	0.507 ug/ml
16) N-HEXATRIACONTANE	20.122	88954	0.406 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
Data File : FE032507.D
Signal(s) : FID1B.CH
Acq On : 03 Aug 2020 20:19
Operator : DD\AJ
Sample : PB130684BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB130684BL

Integration File: autoint1.e
Quant Time: Aug 04 00:48:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
Quant Title :
QLast Update : Wed Jul 29 02:31:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

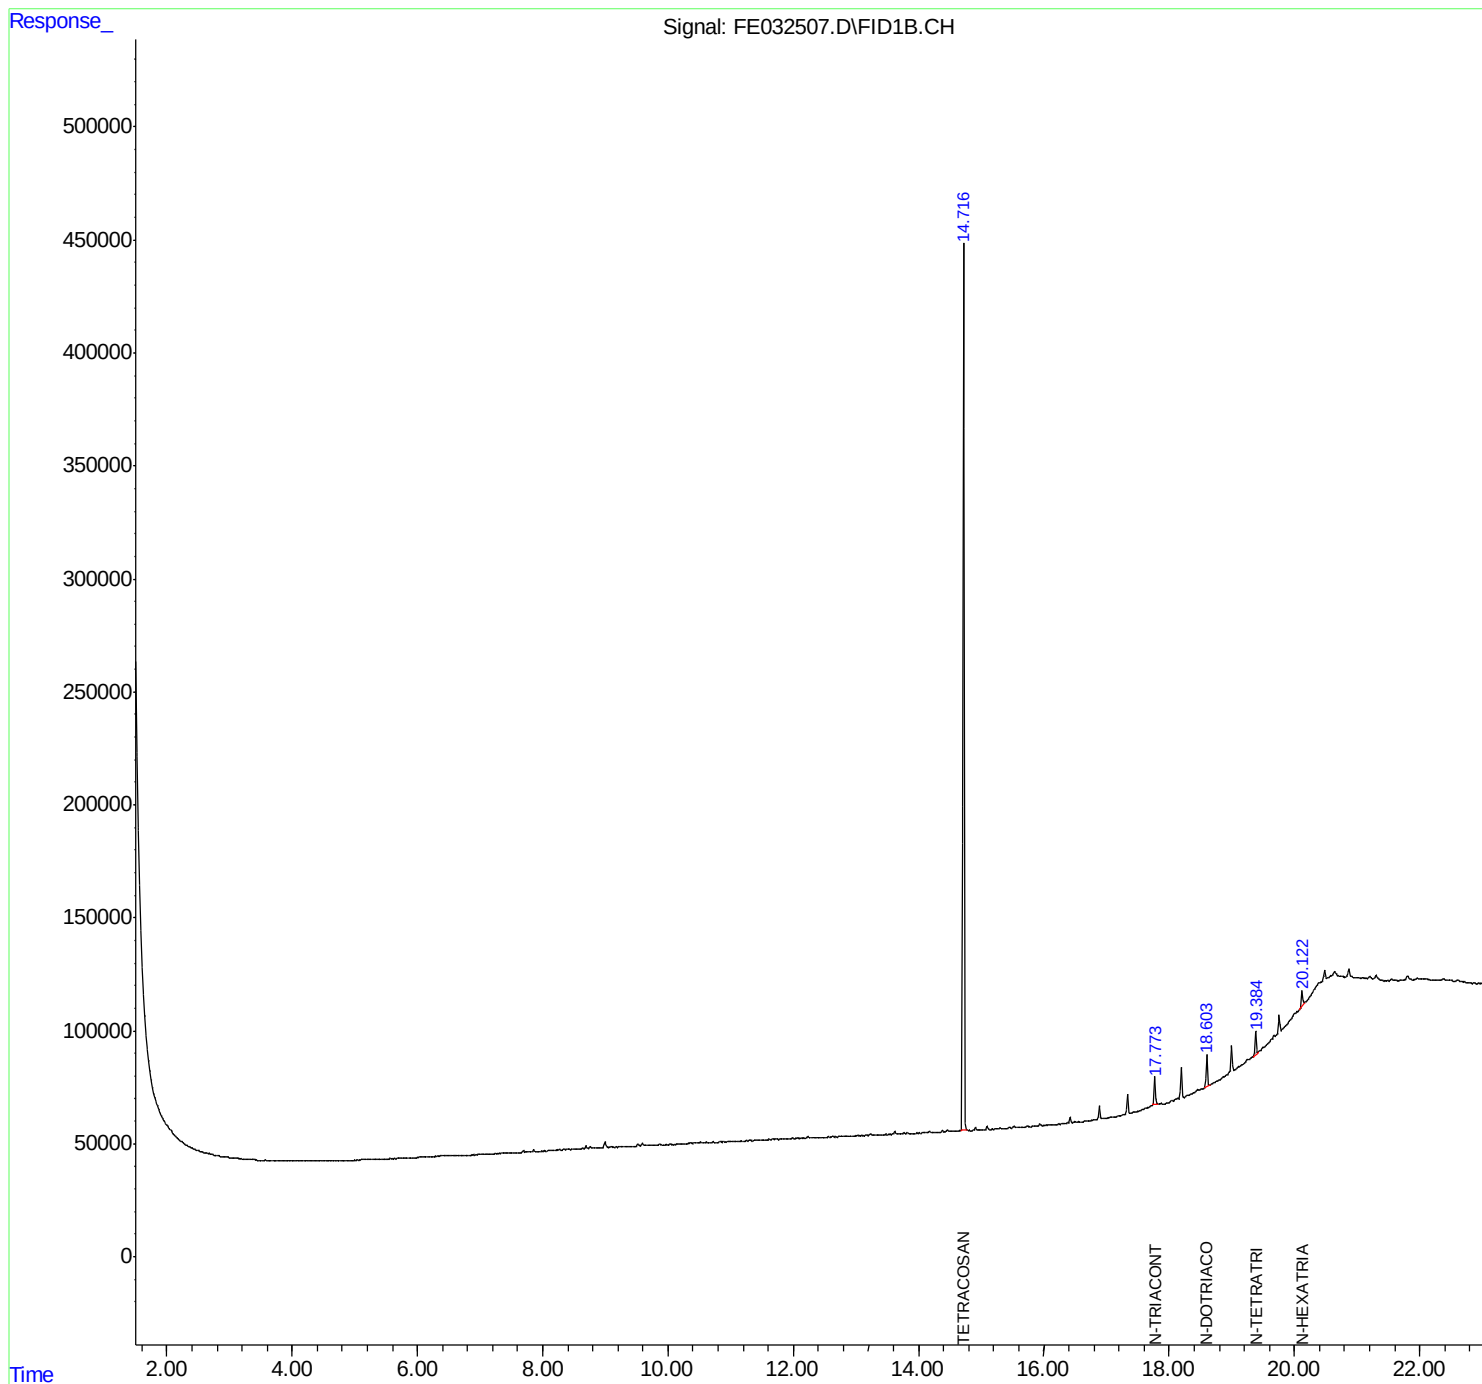


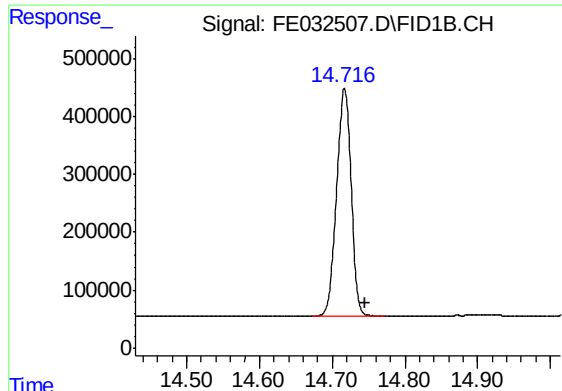

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.717 min
Delta R.T.: -0.028 min
Response: 5436061
Conc: 16.94 ug/ml

Instrument :
FID_E
ClientSampleId :
PB130684BL

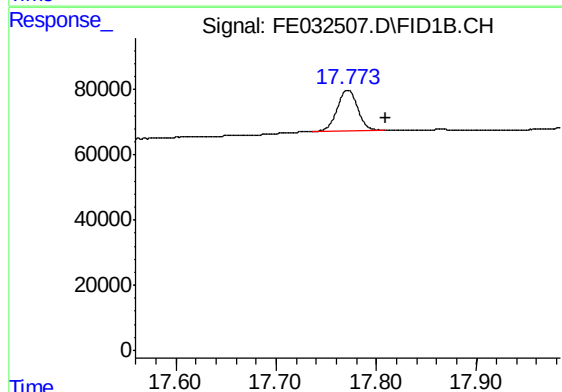


#13 N-TRIACONTANE

R.T.: 17.773 min
Delta R.T.: -0.036 min
Response: 175225
Conc: 0.48 ug/ml

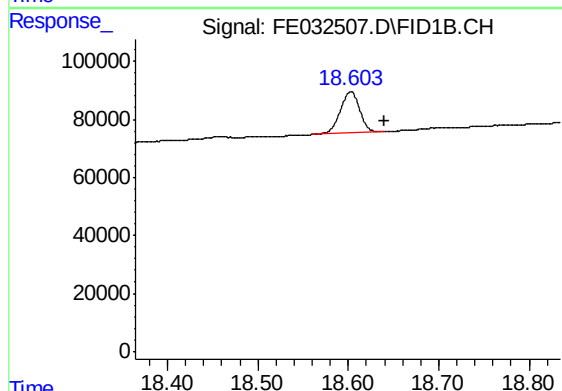


#14 N-DOTRIACONTANE

R.T.: 18.603 min
Delta R.T.: -0.036 min
Response: 208141
Conc: 0.60 ug/ml

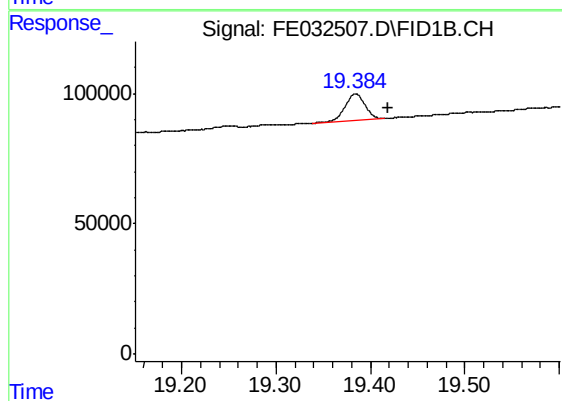

#15 N-TETRATRIACONTANE

R.T.: 19.384 min
Delta R.T.: -0.035 min
Response: 145949
Conc: 0.51 ug/ml

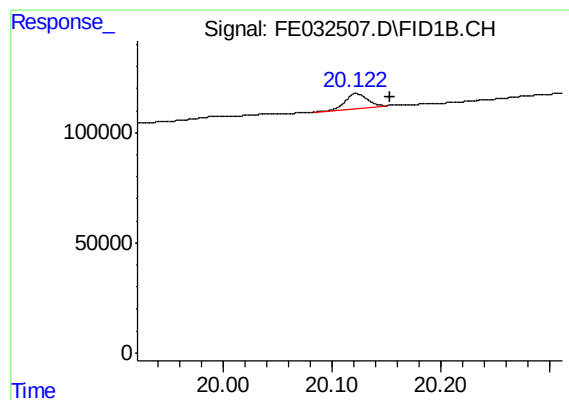

#16 N-HEXATRIACONTANE

R.T.: 20.122 min
Delta R.T.: -0.031 min
Response: 88954
Conc: 0.41 ug/ml

Instrument :
FID_E
ClientSampleId :
PB130684BL