

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
 Data File : FE032509.D
 Signal(s) : FID1B.CH
 Acq On : 03 Aug 2020 21:27
 Operator : DD\AJ
 Sample : PB130692BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 PB130692BL

Integration File: autoint1.e
 Quant Time: Aug 04 00:48:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
 Quant Title :
 QLast Update : Wed Jul 29 02:31:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.718	5543523	17.275 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.883	112659	0.306 ug/ml
13) N-TRIACONTANE	17.769	266051	0.725 ug/ml
14) N-DOTRIACONTANE	18.601	306875	0.888 ug/ml
15) N-TETRATRIACONTANE	19.384	224738	0.781 ug/ml
16) N-HEXATRIACONTANE	20.123	149274	0.681 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
Data File : FE032509.D
Signal(s) : FID1B.CH
Acq On : 03 Aug 2020 21:27
Operator : DD\AJ
Sample : PB130692BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :
PB130692BL

Integration File: autoint1.e
Quant Time: Aug 04 00:48:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
Quant Title :
QLast Update : Wed Jul 29 02:31:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

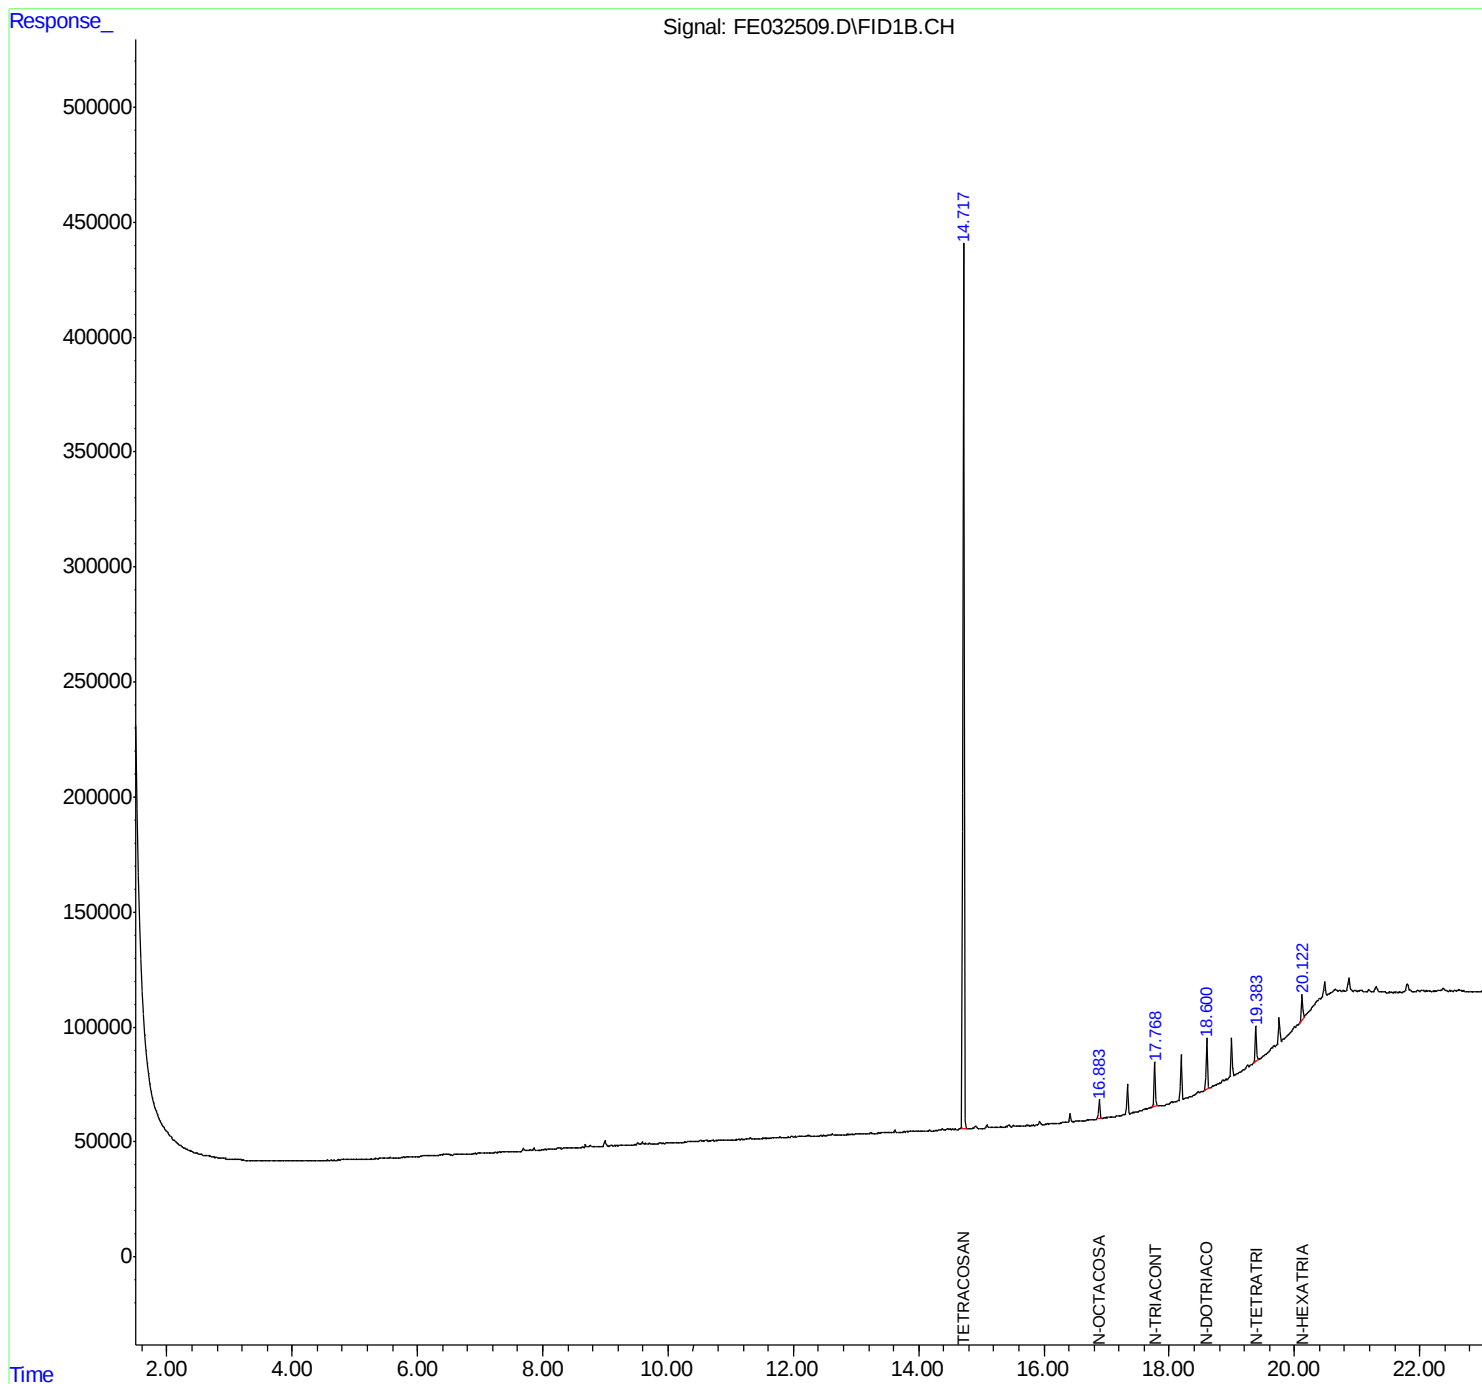


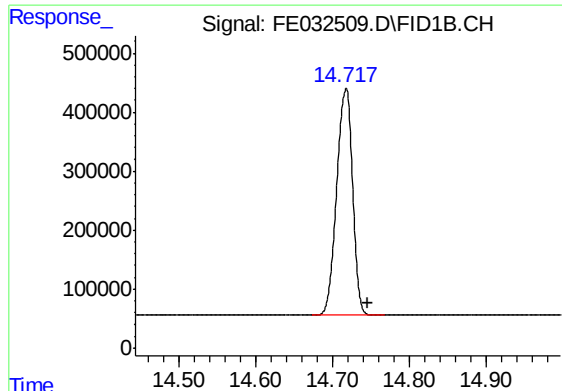

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.718 min
Delta R.T.: -0.027 min
Response: 5543523
Conc: 17.28 ug/ml

Instrument :
FID_E
ClientSampleId :
PB130692BL

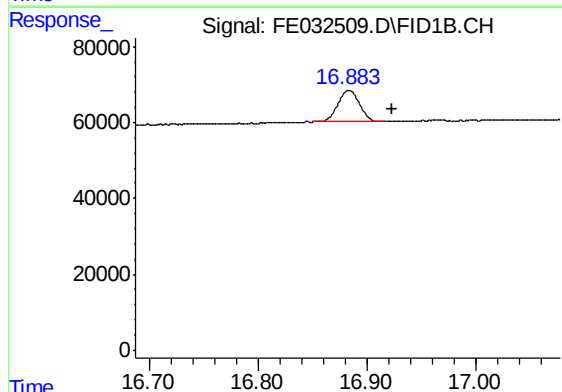


#12 N-OCTACOSANE

R.T.: 16.883 min
Delta R.T.: -0.040 min
Response: 112659
Conc: 0.31 ug/ml

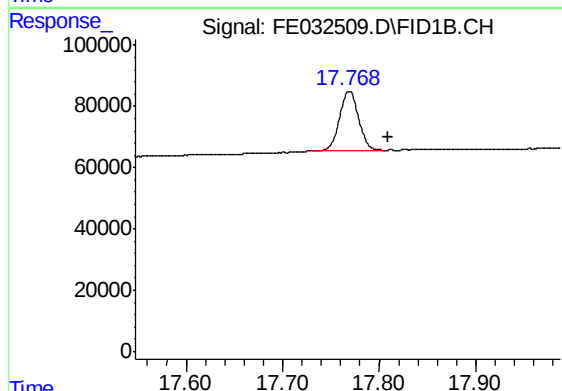


#13 N-TRIACONTANE

R.T.: 17.769 min
Delta R.T.: -0.040 min
Response: 266051
Conc: 0.72 ug/ml

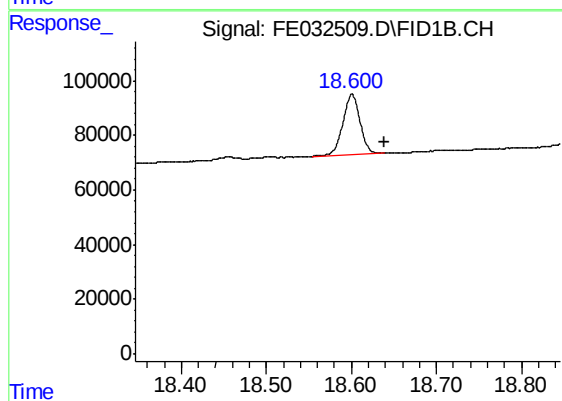

#14 N-DOTRIACONTANE


R.T.: 18.601 min
Delta R.T.: -0.039 min
Response: 306875
Conc: 0.89 ug/ml

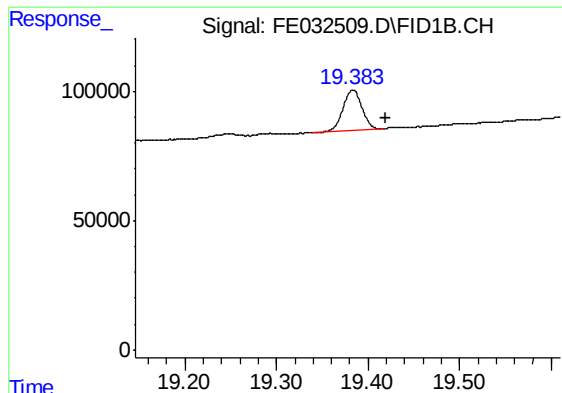

#15 N-TETRATRIACONTANE

R.T.: 19.384 min
Delta R.T.: -0.035 min
Response: 224738
Conc: 0.78 ug/ml

Instrument :
FID_E
ClientSampleId :
PB130692BL

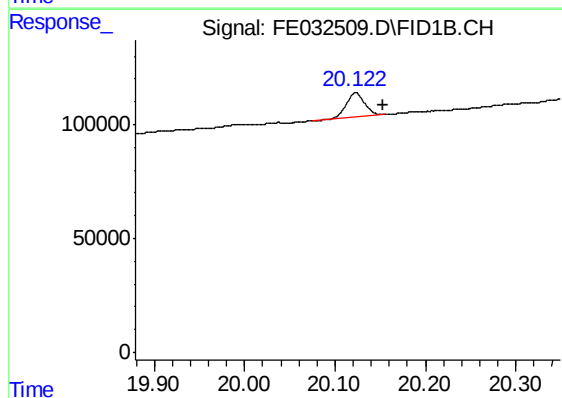

#16 N-HEXATRIACONTANE

R.T.: 20.123 min
Delta R.T.: -0.030 min
Response: 149274
Conc: 0.68 ug/ml