

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
 Data File : FE032512.D
 Signal(s) : FID1B.CH
 Acq On : 03 Aug 2020 23:08
 Operator : DD\AJ
 Sample : L3536-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 JTY1-GW-01

Integration File: autoint1.e
 Quant Time: Aug 04 00:49:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
 Quant Title :
 QLast Update : Wed Jul 29 02:31:52 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.717	6476738	20.184 ug/ml
Target Compounds			
3) N-DODECANE	6.486	1368193	3.766 ug/ml
4) N-TETRADECANE	8.333	1015484	2.800 ug/ml
5) N-HEXADECANE	9.884	562041	1.539 ug/ml
7) N-EICOSANE	12.584f	146289	0.395 ug/ml
13) N-TRIACONTANE	17.769	146708	0.400 ug/ml
14) N-DOTRIACONTANE	18.593	206769	0.598 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
Data File : FE032512.D
Signal(s) : FID1B.CH
Acq On : 03 Aug 2020 23:08
Operator : DD\AJ
Sample : L3536-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JTY1-GW-01

Integration File: autoint1.e
Quant Time: Aug 04 00:49:46 2020
Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
Quant Title :
QLast Update : Wed Jul 29 02:31:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

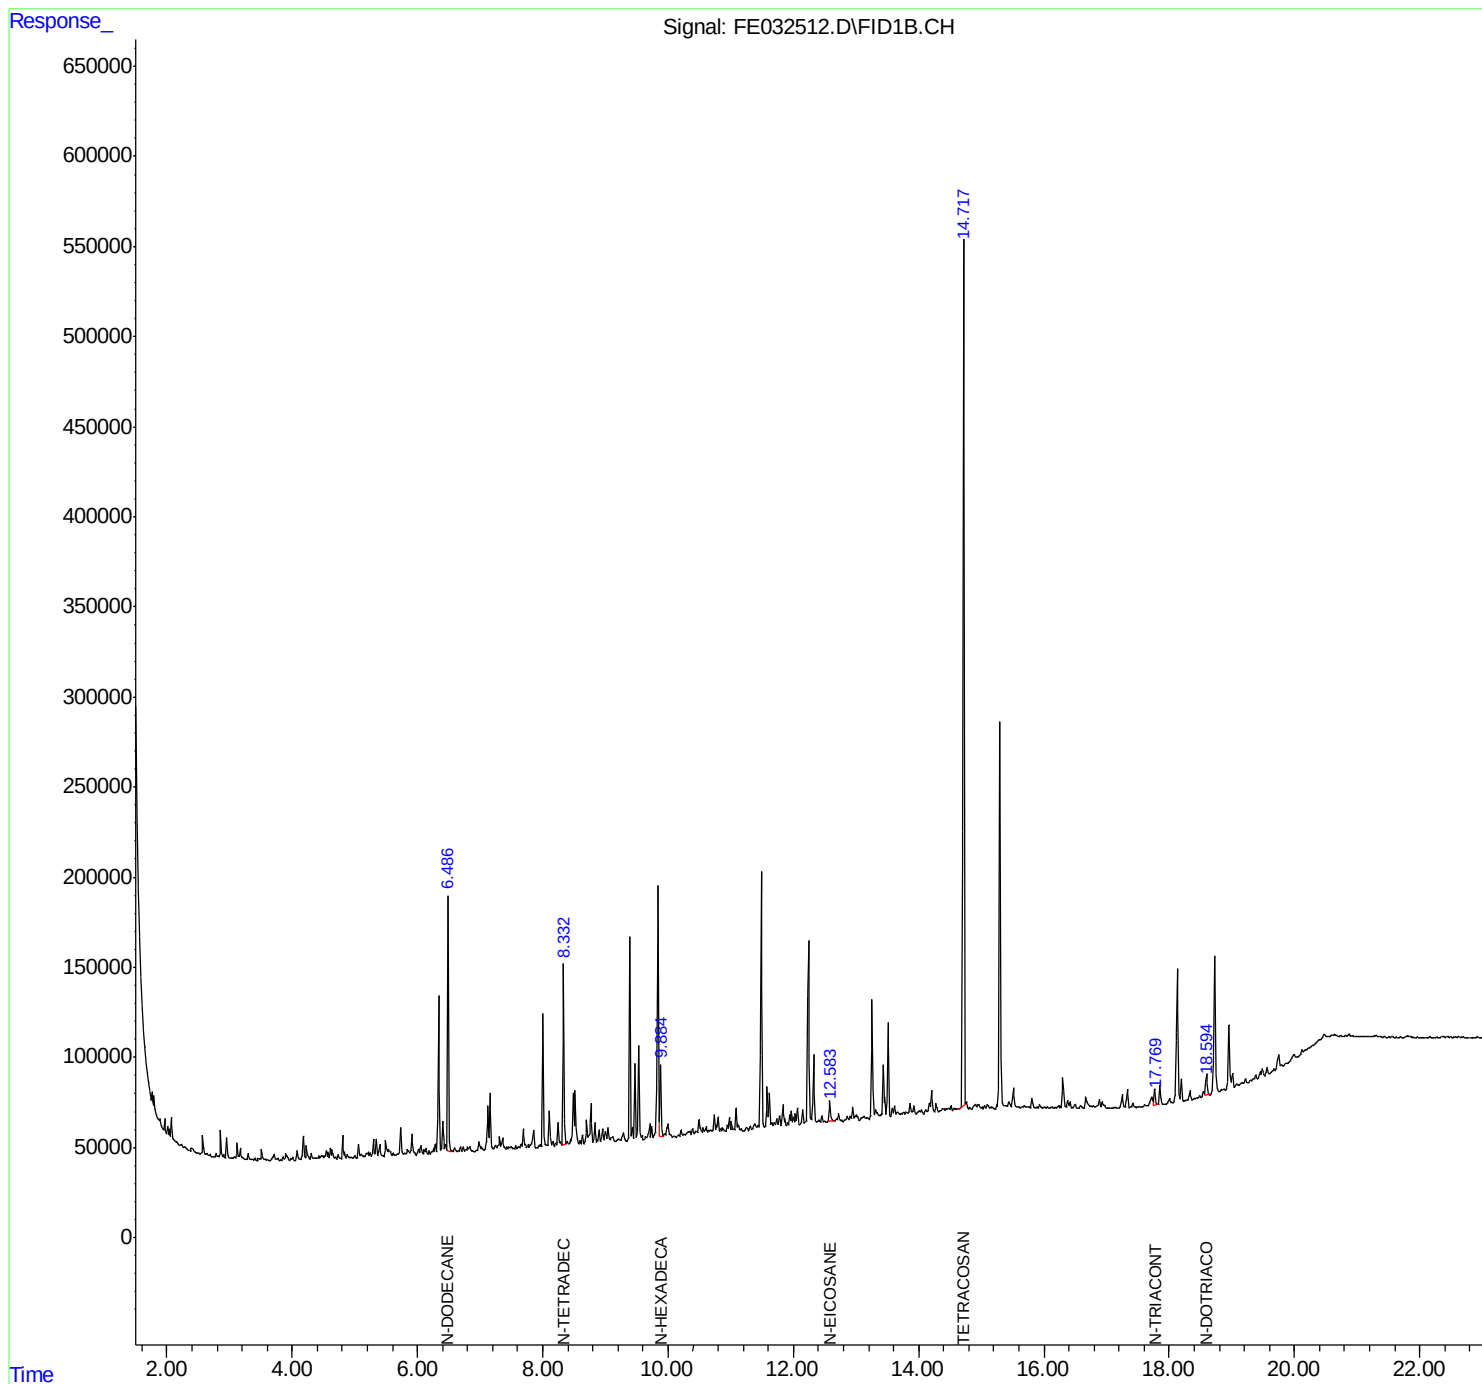


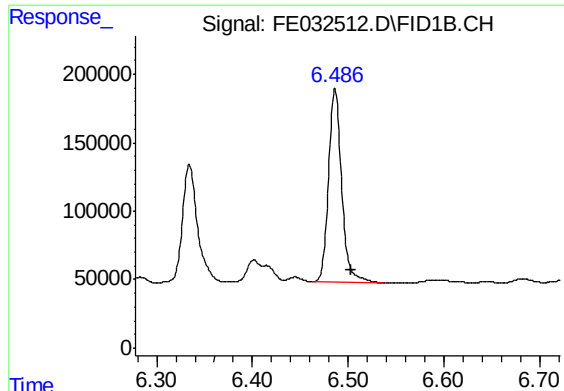

#3 N-DODECANE


R.T.: 6.486 min
Delta R.T.: -0.017 min
Response: 1368193
Conc: 3.77 ug/ml

Instrument :
FID_E
ClientSampleId :
JTY1-GW-01

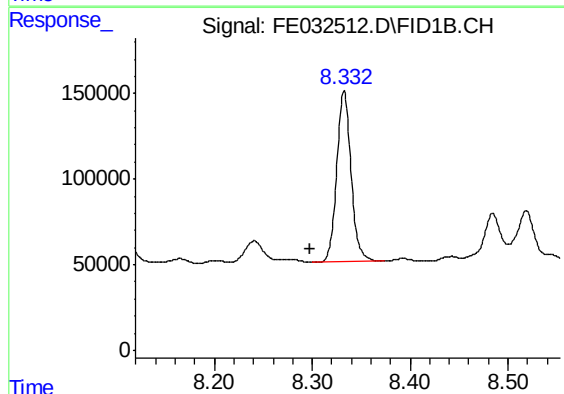


#4 N-TETRADECANE

R.T.: 8.333 min
Delta R.T.: 0.034 min
Response: 1015484
Conc: 2.80 ug/ml

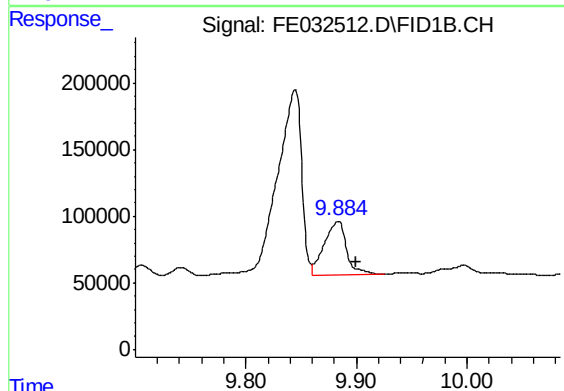


#5 N-HEXADECANE

R.T.: 9.884 min
Delta R.T.: -0.016 min
Response: 562041
Conc: 1.54 ug/ml

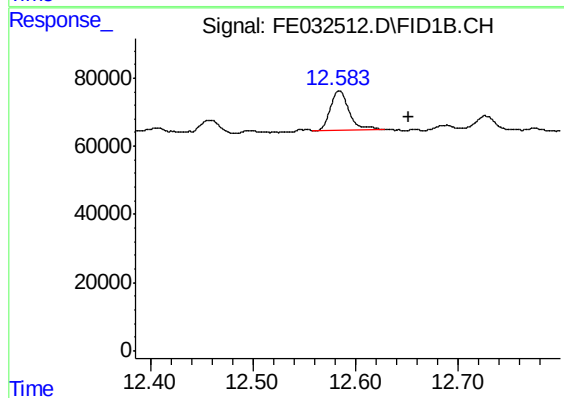

#7 N-EICOSANE


R.T.: 12.584 min
Delta R.T.: -0.068 min
Response: 146289
Conc: 0.40 ug/ml

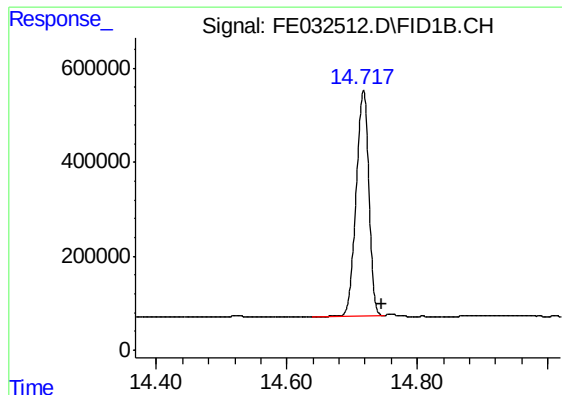

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.717 min
Delta R.T.: -0.028 min
Response: 6476738
Conc: 20.18 ug/ml

Instrument :
FID_E
ClientSampleId :
JTY1-GW-01

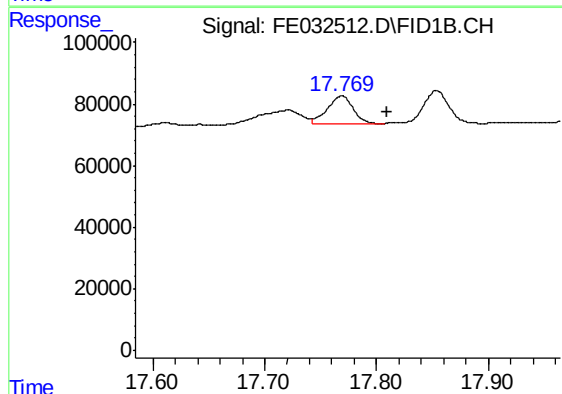

#13 N-TRIACONTANE

R.T.: 17.769 min
Delta R.T.: -0.040 min
Response: 146708
Conc: 0.40 ug/ml

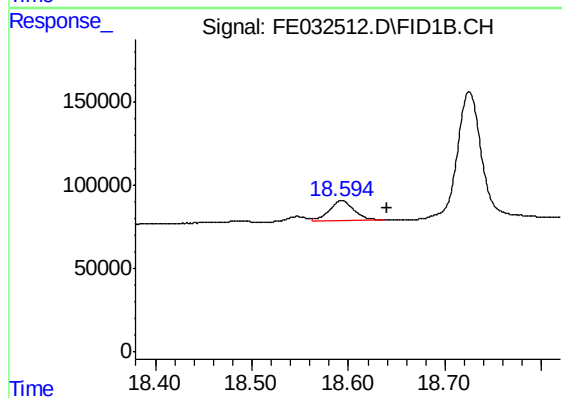

#14 N-DOTRIACONTANE

R.T.: 18.593 min
Delta R.T.: -0.047 min
Response: 206769
Conc: 0.60 ug/ml