

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
Data File : FE032501.D
Signal(s) : FID1B.CH
Acq On : 03 Aug 2020 16:54
Operator : DD\AJ
Sample : L3537-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
JTY1-WC-S-0203

Manual Integrations
APPROVED

Ankita
8/4/2020 12:02:16 PM

Integration File: autoint1.e
Quant Time: Aug 04 00:47:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
Quant Title :
QLast Update : Wed Jul 29 02:31:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.721	7676544	23.923 ug/mlm

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080320\
Data File : FE032501.D
Signal(s) : FID1B.CH
Acq On : 03 Aug 2020 16:54
Operator : DD\AJ
Sample : L3537-02
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
JTY1-WC-S-0203


Manual Integrations
APPROVED

Ankita
8/4/2020 12:02:16 PM

Integration File: autoint1.e
Quant Time: Aug 04 00:47:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072820.M
Quant Title :
QLast Update : Wed Jul 29 02:31:52 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

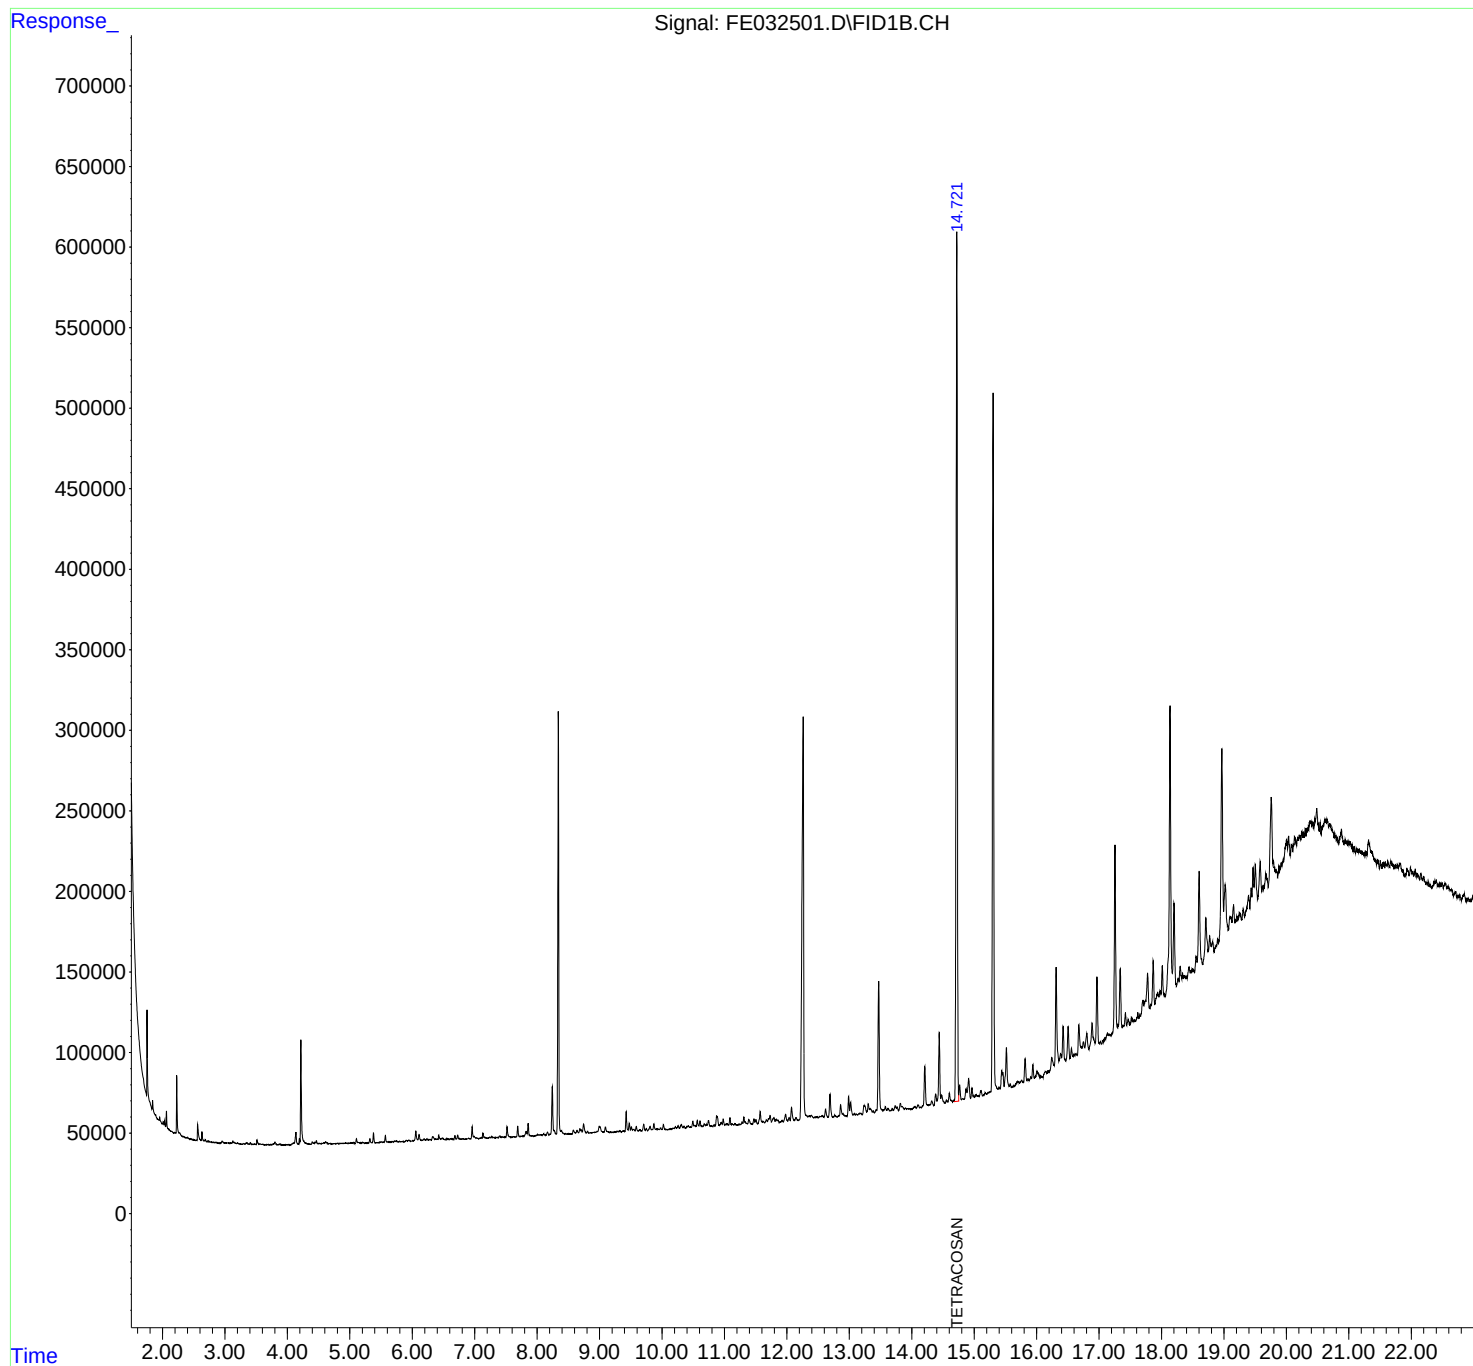

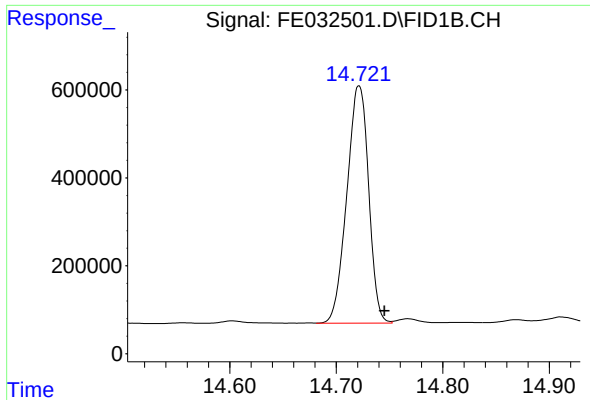

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.721 min
Delta R.T.: -0.024 min
Response: 7676544
Conc: 23.92 ug/ml m

Instrument :
FID_E
ClientSampleId :
JTY1-WC-S-0203

Manual Integrations
APPROVED

Ankita
8/4/2020 12:02:16 PM