

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080323AL\
 Data File : FE043662.D
 Signal(s) : FID1B.ch
 Acq On : 02 Aug 2023 06:29
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 02 10:59:24 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 080323.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 02 09:56:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

11) T	n-Heneicosane (C21)	13.584	363084	2.051 ug/ml
13) T	n-Docosane (C22)	14.123	642111	3.661 ug/ml
14) T	n-Tetracosane (C24)	15.261	152287	0.867 ug/ml
15) T	n-Hexacosane (C26)	16.317f	553001	3.200 ug/ml
17) T	n-Tricontane (C30)	18.104	159875	0.965 ug/ml
18) T	n-Dotriacontane (C32)	18.985f	175008	1.108 ug/ml
19) T	n-Tetratriacontane (C34)	19.728	159443	1.073 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080323AL\
Data File : FE043662.D
Signal(s) : FID1B.ch
Acq On : 02 Aug 2023 06:29
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 02 10:59:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 080323.M
Quant Title : GC Extractables
QLast Update : Wed Aug 02 09:56:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

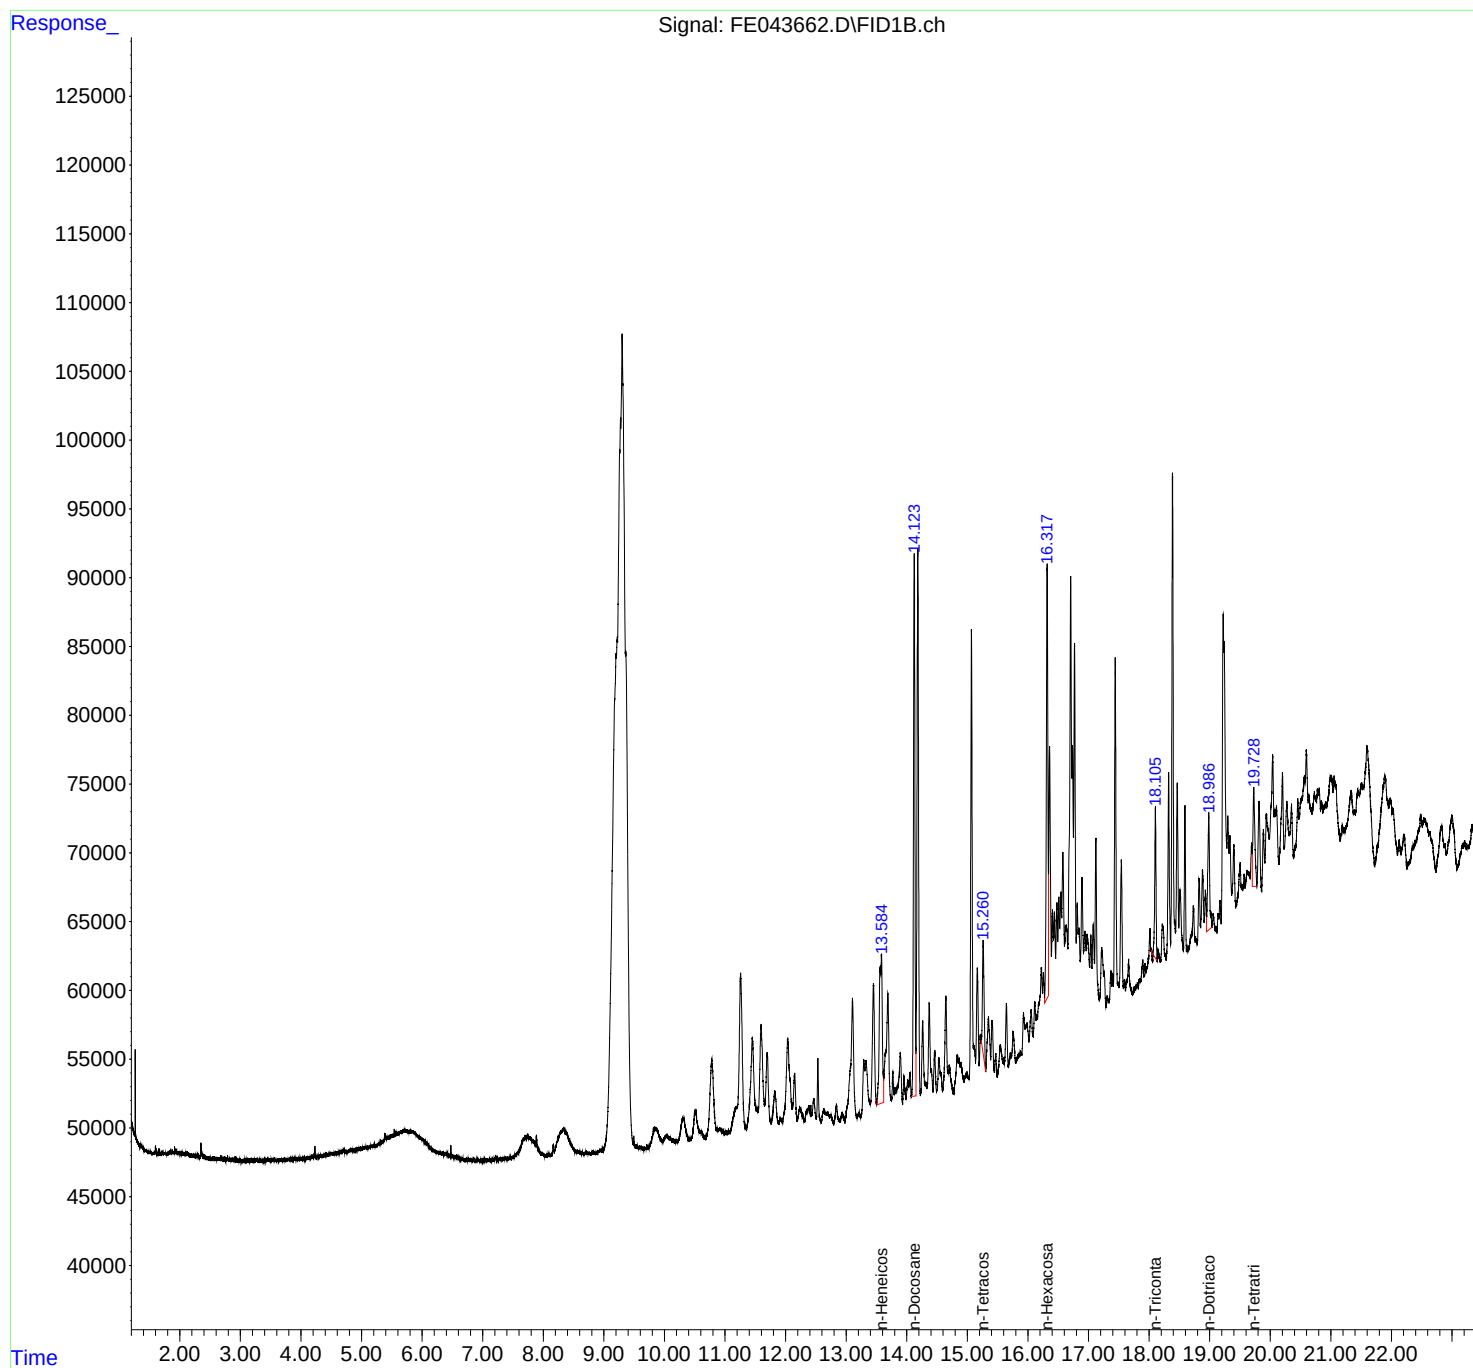


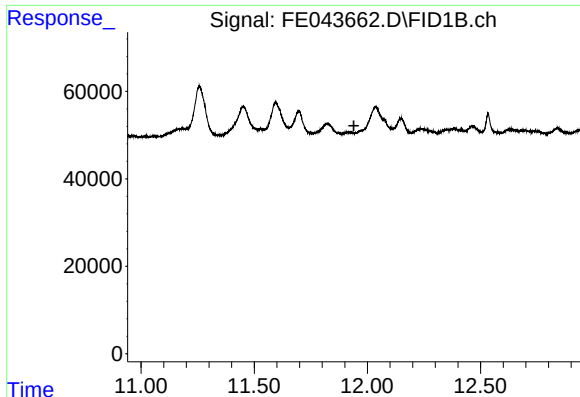

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.940 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

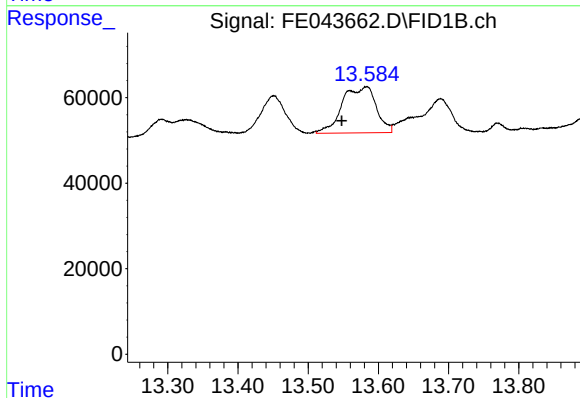


#11 n-Heneicosane (C21)

R.T.: 13.584 min
Delta R.T.: 0.036 min
Response: 363084
Conc: 2.05 ug/ml

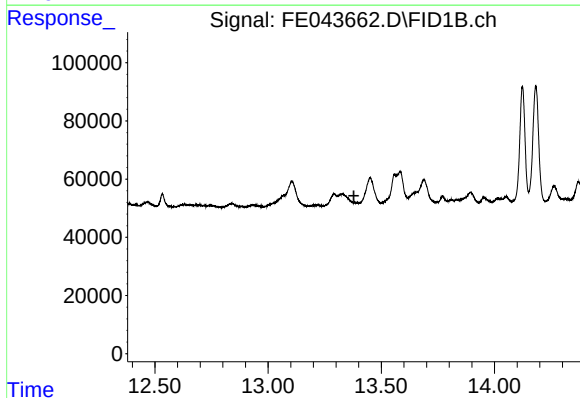


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.379 min
Response: 0
Conc: N.D.

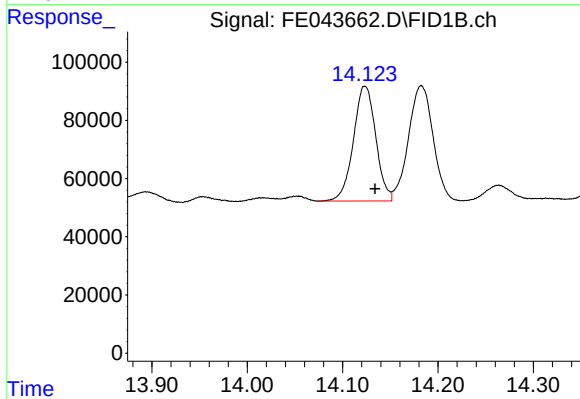

#13 n-Docosane (C22)


R.T.: 14.123 min
Delta R.T.: -0.011 min
Response: 642111
Conc: 3.66 ug/ml

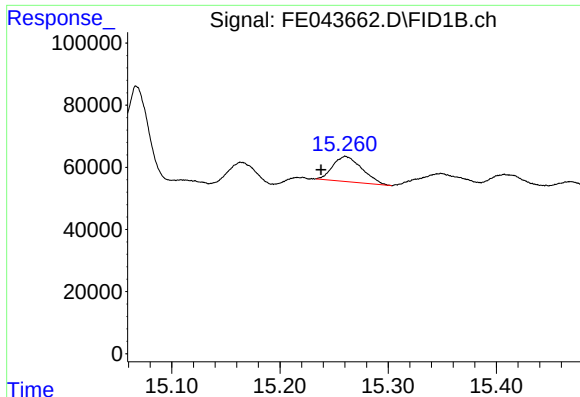

#14 n-Tetracosane (C24)


R.T.: 15.261 min
Delta R.T.: 0.023 min
Response: 152287
Conc: 0.87 ug/ml

Instrument :
FID_E
ClientSampleId :

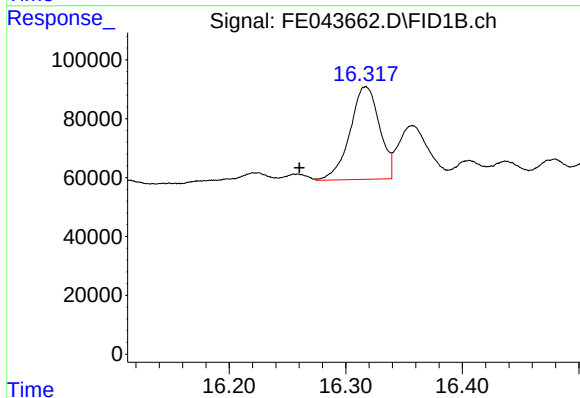


#15 n-Hexacosane (C26)

R.T.: 16.317 min
Delta R.T.: 0.057 min
Response: 553001
Conc: 3.20 ug/ml

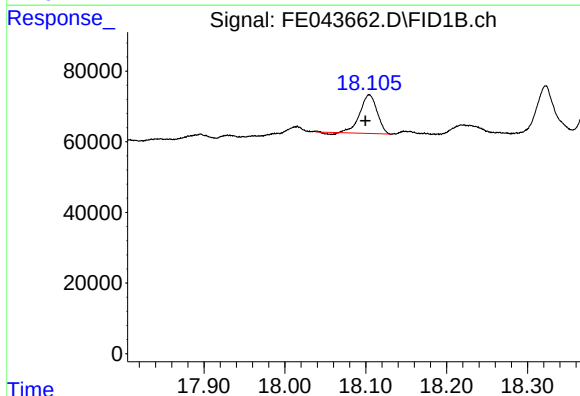


#17 n-Tricontane (C30)

R.T.: 18.104 min
Delta R.T.: 0.005 min
Response: 159875
Conc: 0.97 ug/ml

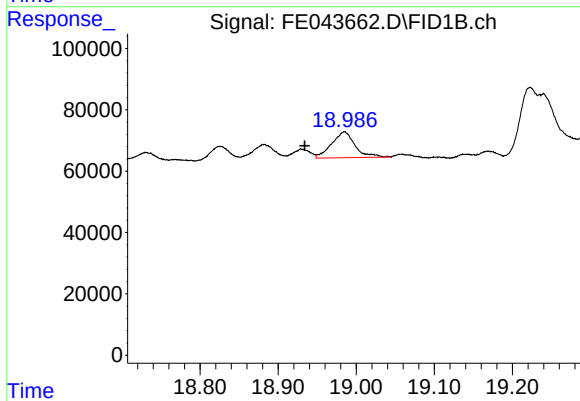

#18 n-Dotriacontane (C32)

R.T.: 18.985 min
Delta R.T.: 0.051 min
Response: 175008
Conc: 1.11 ug/ml

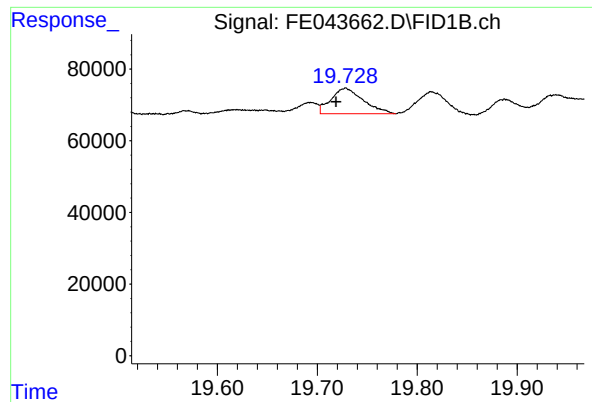

#19 n-Tetratriacontane (C34)

R.T.: 19.728 min
Delta R.T.: 0.010 min
Response: 159443
Conc: 1.07 ug/ml

Instrument :
FID_E
ClientSampleId :