

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080323AL\
 Data File : FE043692.D
 Signal(s) : FID1B.ch
 Acq On : 02 Aug 2023 21:40
 Operator : YP\AJ
 Sample : 03854-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 03 01:42:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 080323.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 02 09:56:52 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.943	4361502	21.165 ug/ml
Spiked Amount 50.000		Recovery =	42.33%
12) S 1-chlorooctadecane (S...	13.382	3313394	21.233 ug/ml
Spiked Amount 50.000		Recovery =	42.47%
Target Compounds			
1) T n-Nonane (C9)	3.273f	84435	0.523 ug/ml
10) T n-Eicosane (C20)	12.986f	251085	1.419 ug/ml
11) T n-Heneicosane (C21)	13.556	117409	0.663 ug/ml
14) T n-Tetracosane (C24)	15.203	132380	0.753 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080323AL\
Data File : FE043692.D
Signal(s) : FID1B.ch
Acq On : 02 Aug 2023 21:40
Operator : YP\AJ
Sample : 03854-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 03 01:42:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 080323.M
Quant Title : GC Extractables
QLast Update : Wed Aug 02 09:56:52 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 uL
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

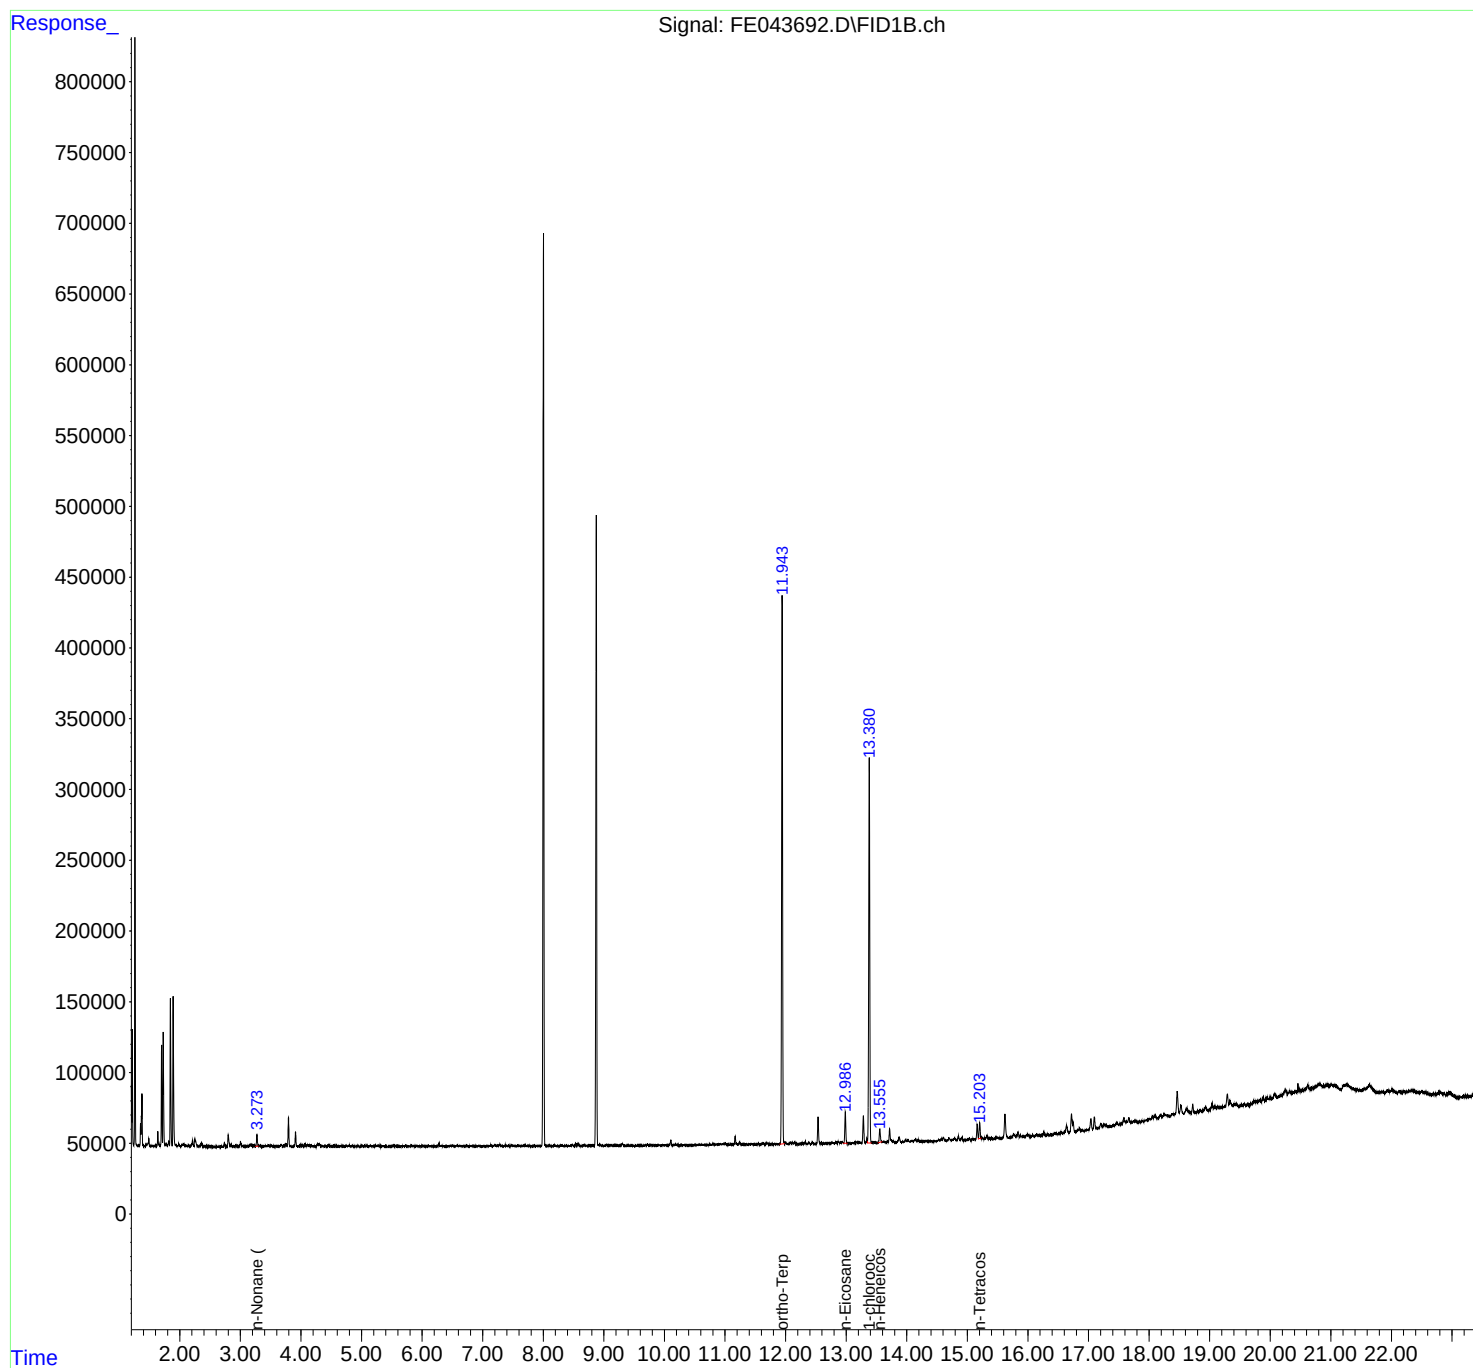


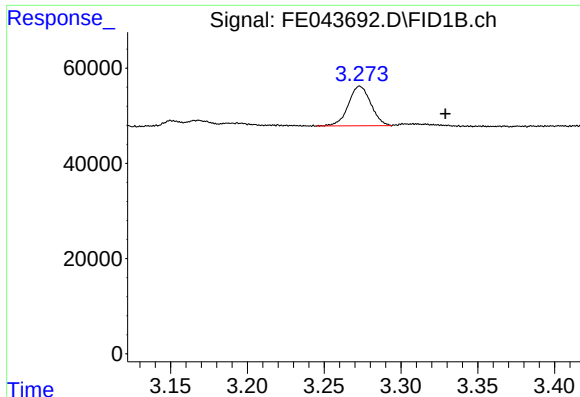

#1 n-Nonane (C9)


R.T.: 3.273 min
Delta R.T.: -0.056 min
Response: 84435
Conc: 0.52 ug/ml

Instrument :
FID_E
ClientSampleId :

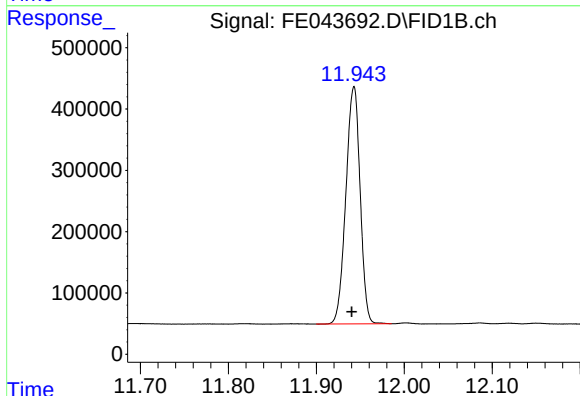


#9 ortho-Terphenyl (SURR)

R.T.: 11.943 min
Delta R.T.: 0.003 min
Response: 4361502
Conc: 21.16 ug/ml

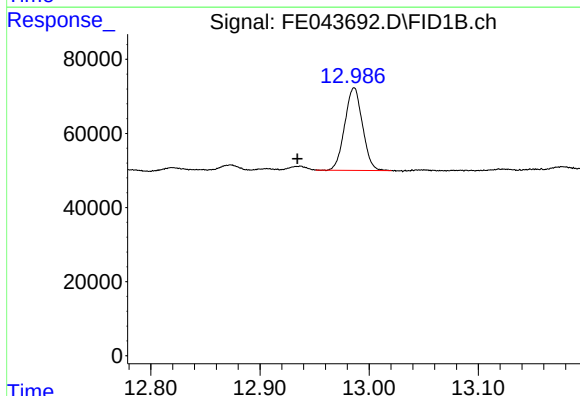


#10 n-Eicosane (C20)

R.T.: 12.986 min
Delta R.T.: 0.052 min
Response: 251085
Conc: 1.42 ug/ml

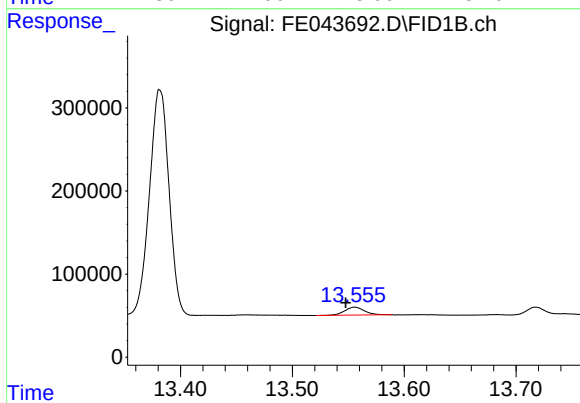

#11 n-Heneicosane (C21)


R.T.: 13.556 min
Delta R.T.: 0.008 min
Response: 117409
Conc: 0.66 ug/ml

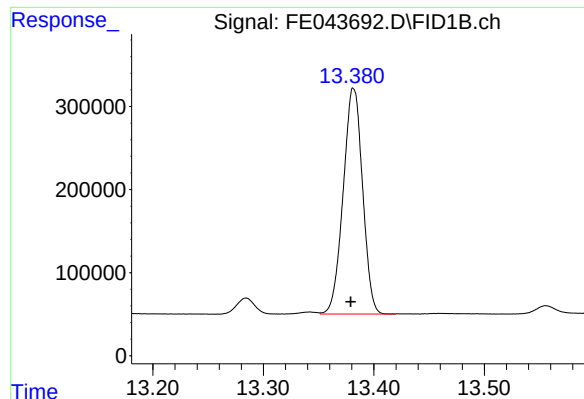

#12 1-chlorooctadecane (SURR)

R.T.: 13.382 min
Delta R.T.: 0.003 min
Response: 3313394
Conc: 21.23 ug/ml

Instrument :
FID_E
ClientSampleId :

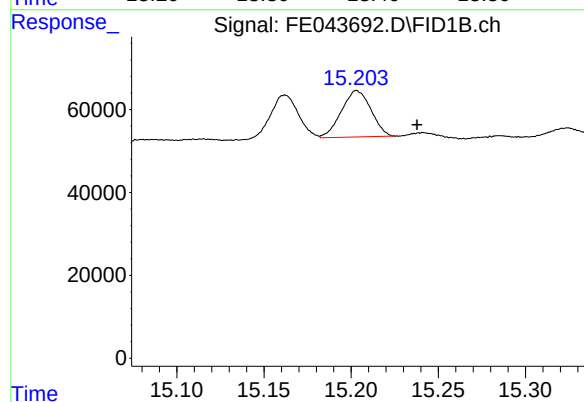

#14 n-Tetracosane (C24)

R.T.: 15.203 min
Delta R.T.: -0.034 min
Response: 132380
Conc: 0.75 ug/ml