

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080422AL\
 Data File : FE036856.D
 Signal(s) : FID1B.ch
 Acq On : 04 Aug 2022 08:18
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 05 04:07:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071722.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 18 02:35:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.813	95852	0.563 ug/ml
11) T n-Heneicosane (C21)	13.433	131705	0.770 ug/ml
13) T n-Docosane (C22)	14.021	109779	0.643 ug/ml
14) T n-Tetracosane (C24)	15.098	1159751	6.804 ug/ml
15) T n-Hexacosane (C26)	16.150	66009	0.395 ug/ml
16) T n-Octacosane (C28)	17.101	51790	0.317 ug/ml
17) T n-Tricontane (C30)	17.990	49587	0.326 ug/ml
18) T n-Dotriacontane (C32)	18.814	188501	1.567 ug/ml
19) T n-Tetratriacontane (C34)	19.607	51899	0.623 ug/ml
20) T n-Hexatriacontane (C36)	20.354	185379	3.157 ug/ml
21) T n-Octatriacontane (C38)	21.065	244243	4.871 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080422AL\
Data File : FE036856.D
Signal(s) : FID1B.ch
Acq On : 04 Aug 2022 08:18
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 05 04:07:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071722.M
Quant Title : GC Extractables
QLast Update : Mon Jul 18 02:35:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

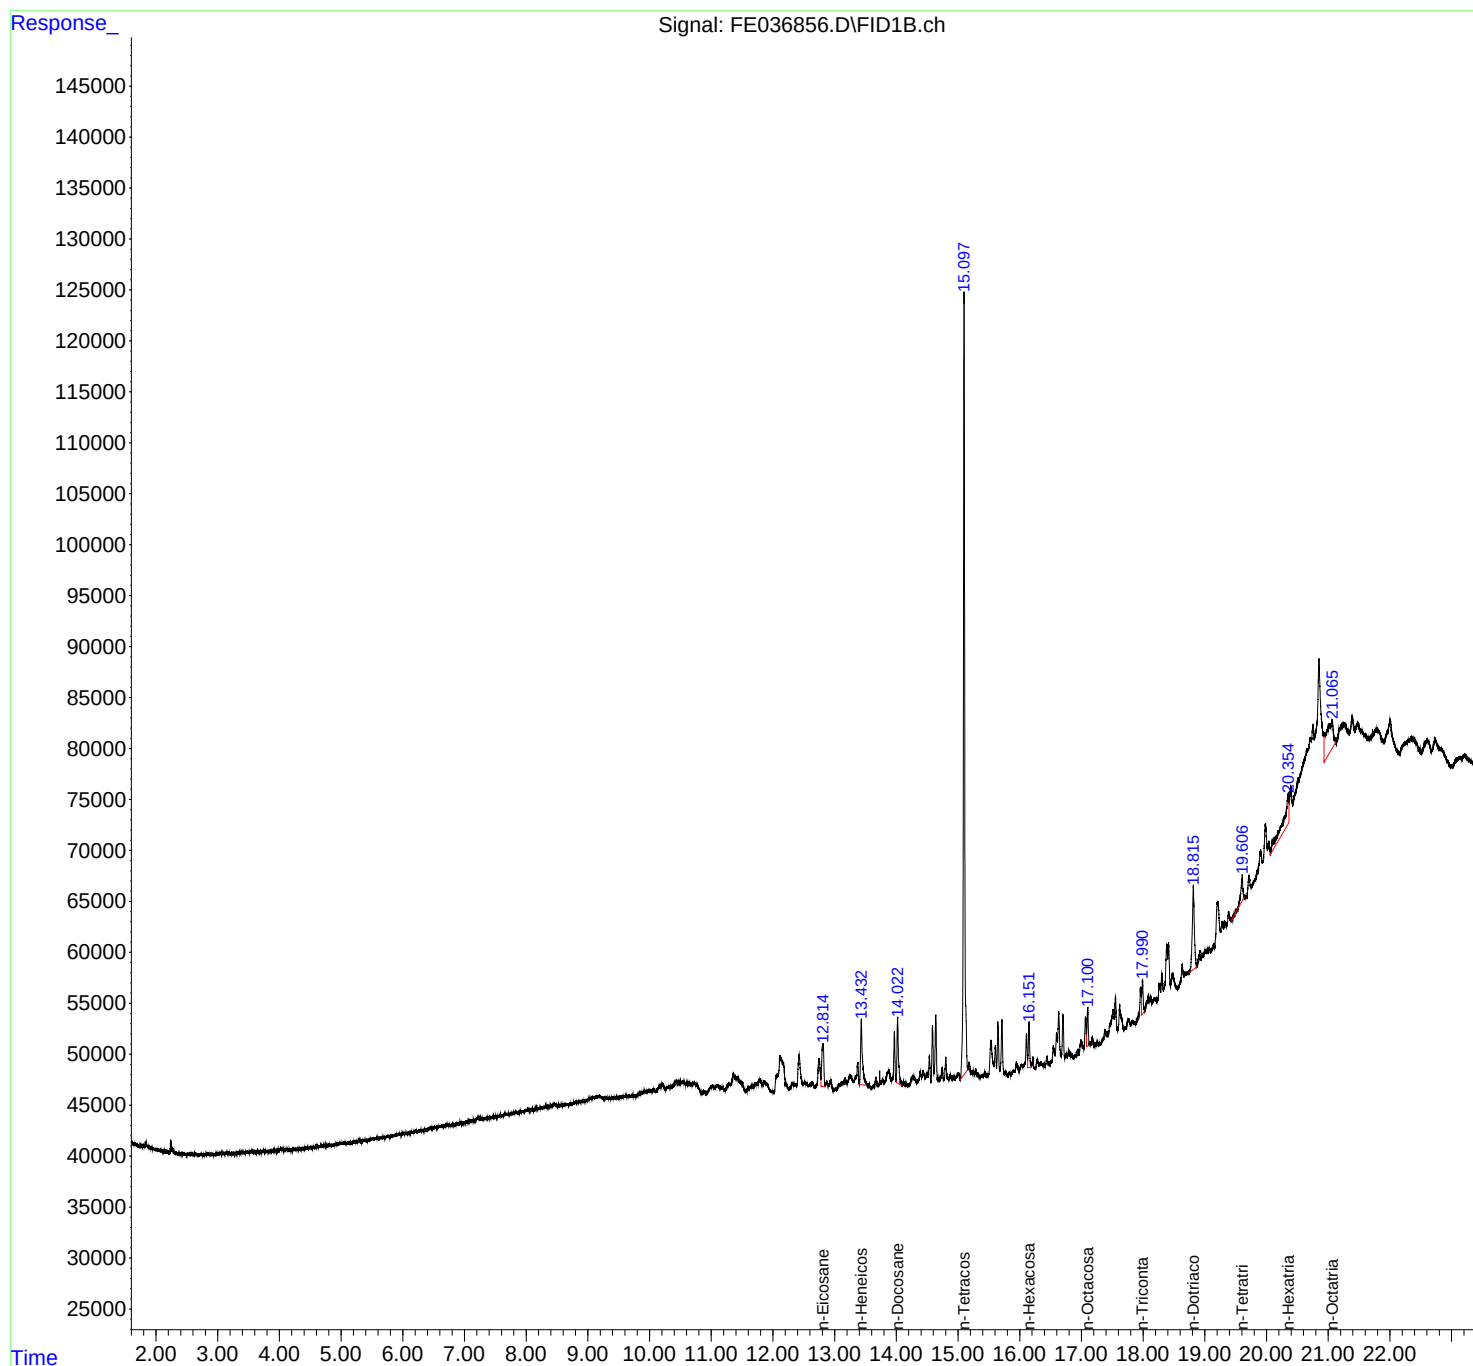


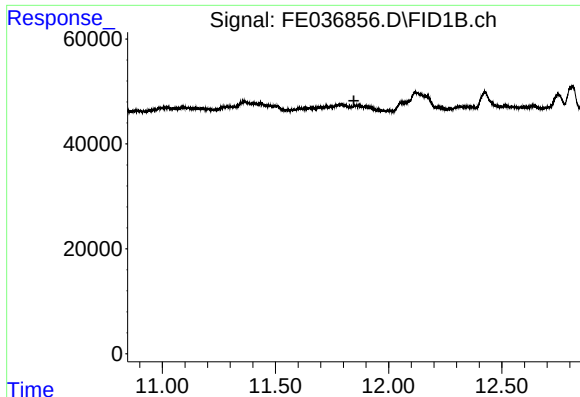

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.846 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

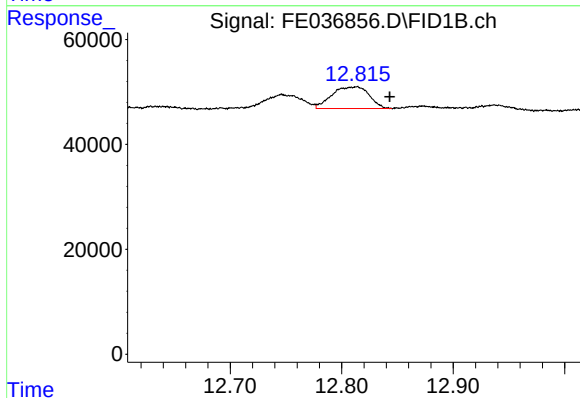


#10 n-Eicosane (C20)

R.T.: 12.813 min
Delta R.T.: -0.030 min
Response: 95852
Conc: 0.56 ug/ml

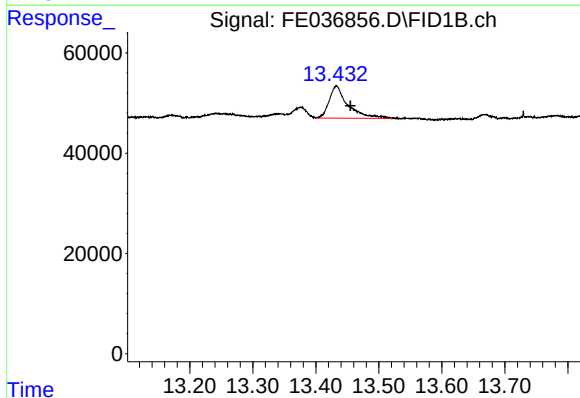


#11 n-Heneicosane (C21)

R.T.: 13.433 min
Delta R.T.: -0.022 min
Response: 131705
Conc: 0.77 ug/ml

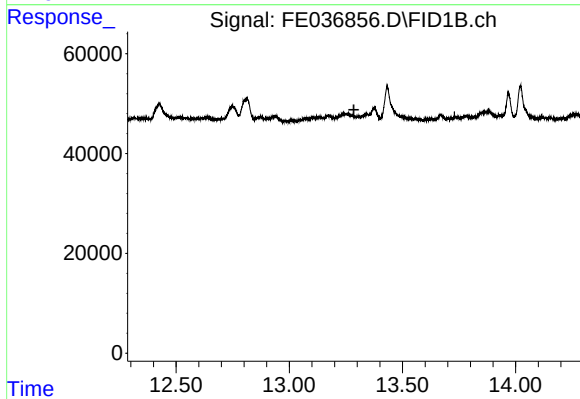

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.286 min
Response: 0
Conc: N.D.

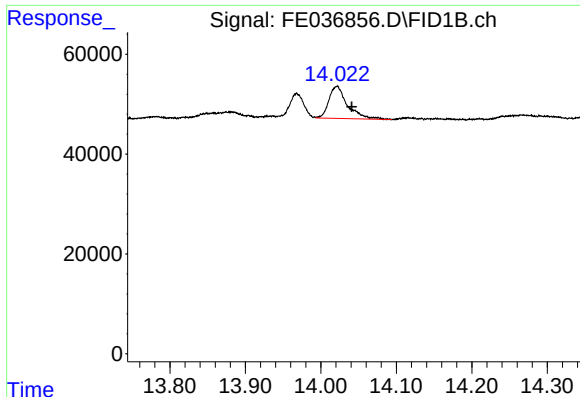

#13 n-Docosane (C22)


R.T.: 14.021 min
Delta R.T.: -0.020 min
Response: 109779
Conc: 0.64 ug/ml

Instrument :
FID_E
ClientSampleId :

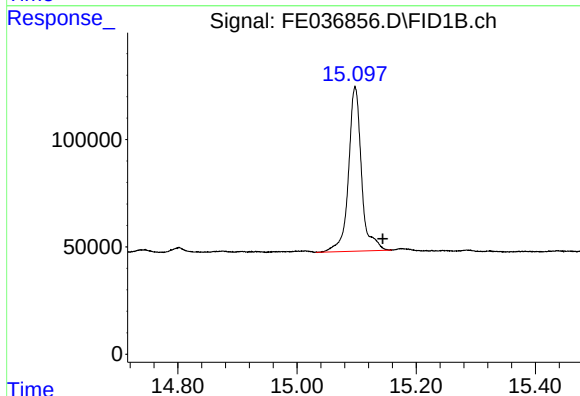


#14 n-Tetracosane (C24)

R.T.: 15.098 min
Delta R.T.: -0.046 min
Response: 1159751
Conc: 6.80 ug/ml

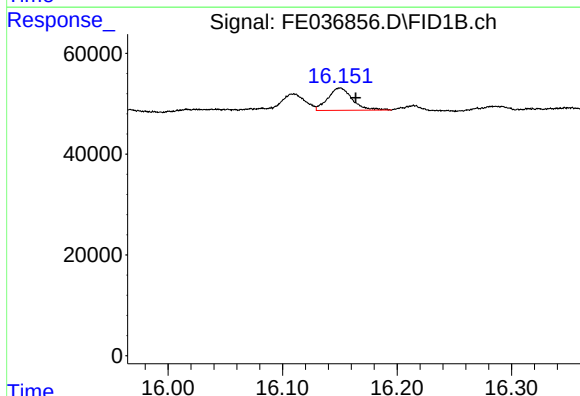


#15 n-Hexacosane (C26)

R.T.: 16.150 min
Delta R.T.: -0.014 min
Response: 66009
Conc: 0.39 ug/ml

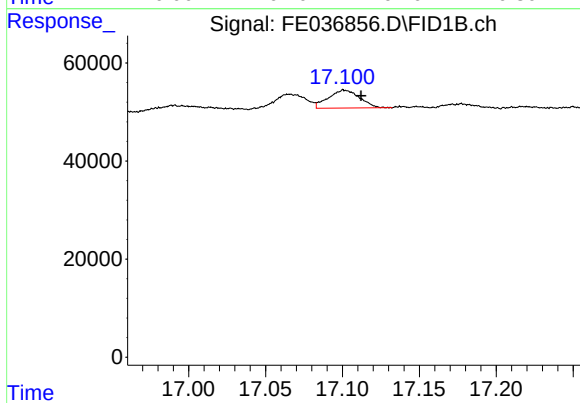

#16 n-Octacosane (C28)


R.T.: 17.101 min
Delta R.T.: -0.011 min
Response: 51790
Conc: 0.32 ug/ml

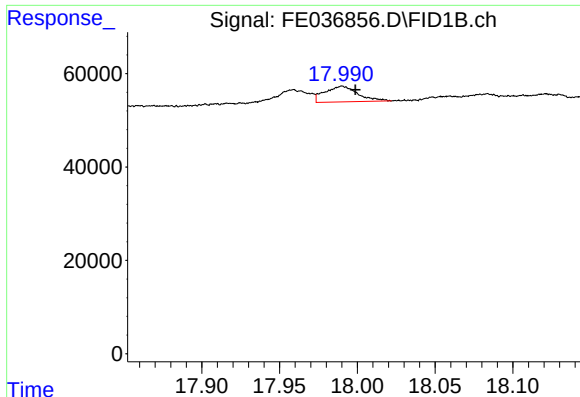

#17 n-Tricontane (C30)


R.T.: 17.990 min
Delta R.T.: -0.009 min
Response: 49587
Conc: 0.33 ug/ml

Instrument :
FID_E
ClientSampleId :

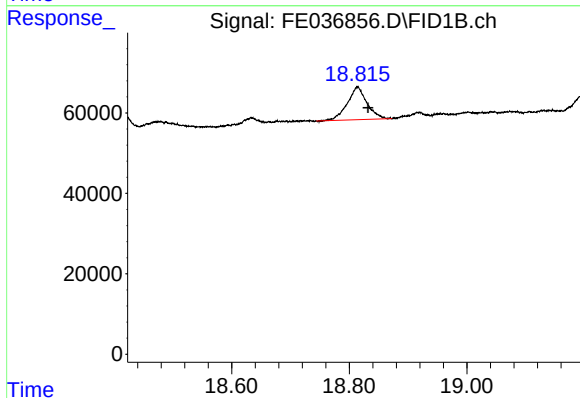


#18 n-Dotriacontane (C32)

R.T.: 18.814 min
Delta R.T.: -0.018 min
Response: 188501
Conc: 1.57 ug/ml

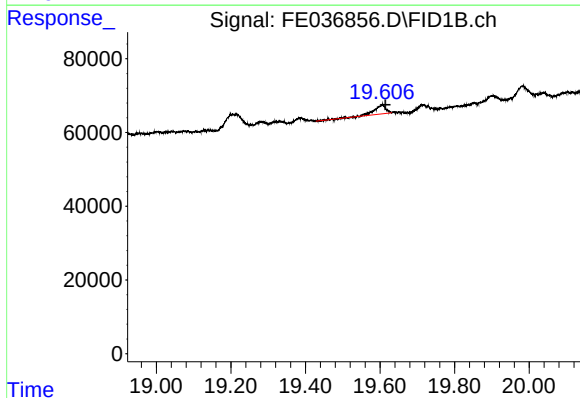


#19 n-Tetratriacontane (C34)

R.T.: 19.607 min
Delta R.T.: -0.008 min
Response: 51899
Conc: 0.62 ug/ml

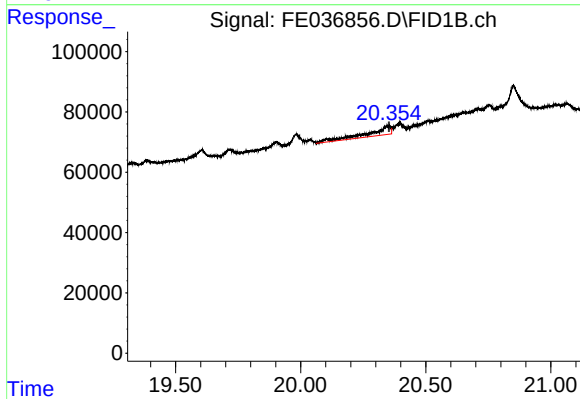

#20 n-Hexatriacontane (C36)

R.T.: 20.354 min
Delta R.T.: 0.000 min
Response: 185379
Conc: 3.16 ug/ml

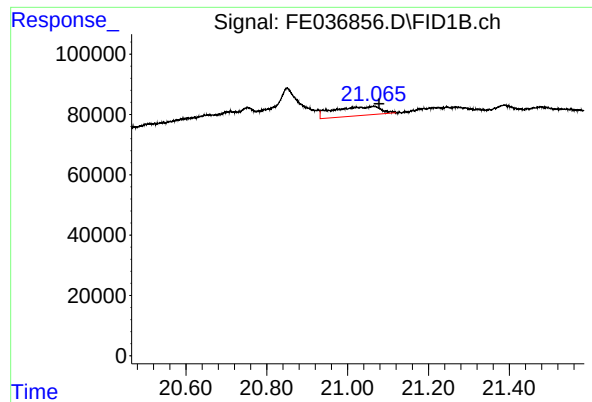

#21 n-Octatriacontane (C38)

R.T.: 21.065 min
Delta R.T.: -0.013 min
Response: 244243
Conc: 4.87 ug/ml

Instrument :
FID_E
ClientSampleId :