

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080422AL\
 Data File : FE036862.D
 Signal(s) : FID1B.ch
 Acq On : 04 Aug 2022 11:41
 Operator : YP\AJ
 Sample : N4016-04DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Aug 05 04:10:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071722.M
 Quant Title : GC Extractables
 QLast Update : Mon Jul 18 02:35:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.831	1175296	6.310 ug/ml
Spiked Amount 50.000		Recovery =	12.62%
12) S 1-chlorooctadecane (S...	13.271	954952	6.277 ug/ml
Spiked Amount 50.000		Recovery =	12.55%
Target Compounds			
10) T n-Eicosane (C20)	12.882	373089	2.193 ug/ml
14) T n-Tetracosane (C24)	15.101	239337	1.404 ug/ml
16) T n-Octacosane (C28)	17.101	48536	0.297 ug/ml
17) T n-Tricontane (C30)	17.985	63932	0.421 ug/ml
19) T n-Tetratriacontane (C34)	19.606	26947	0.324 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080422AL\
Data File : FE036862.D
Signal(s) : FID1B.ch
Acq On : 04 Aug 2022 11:41
Operator : YP\AJ
Sample : N4016-04DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 05 04:10:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 071722.M
Quant Title : GC Extractables
QLast Update : Mon Jul 18 02:35:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

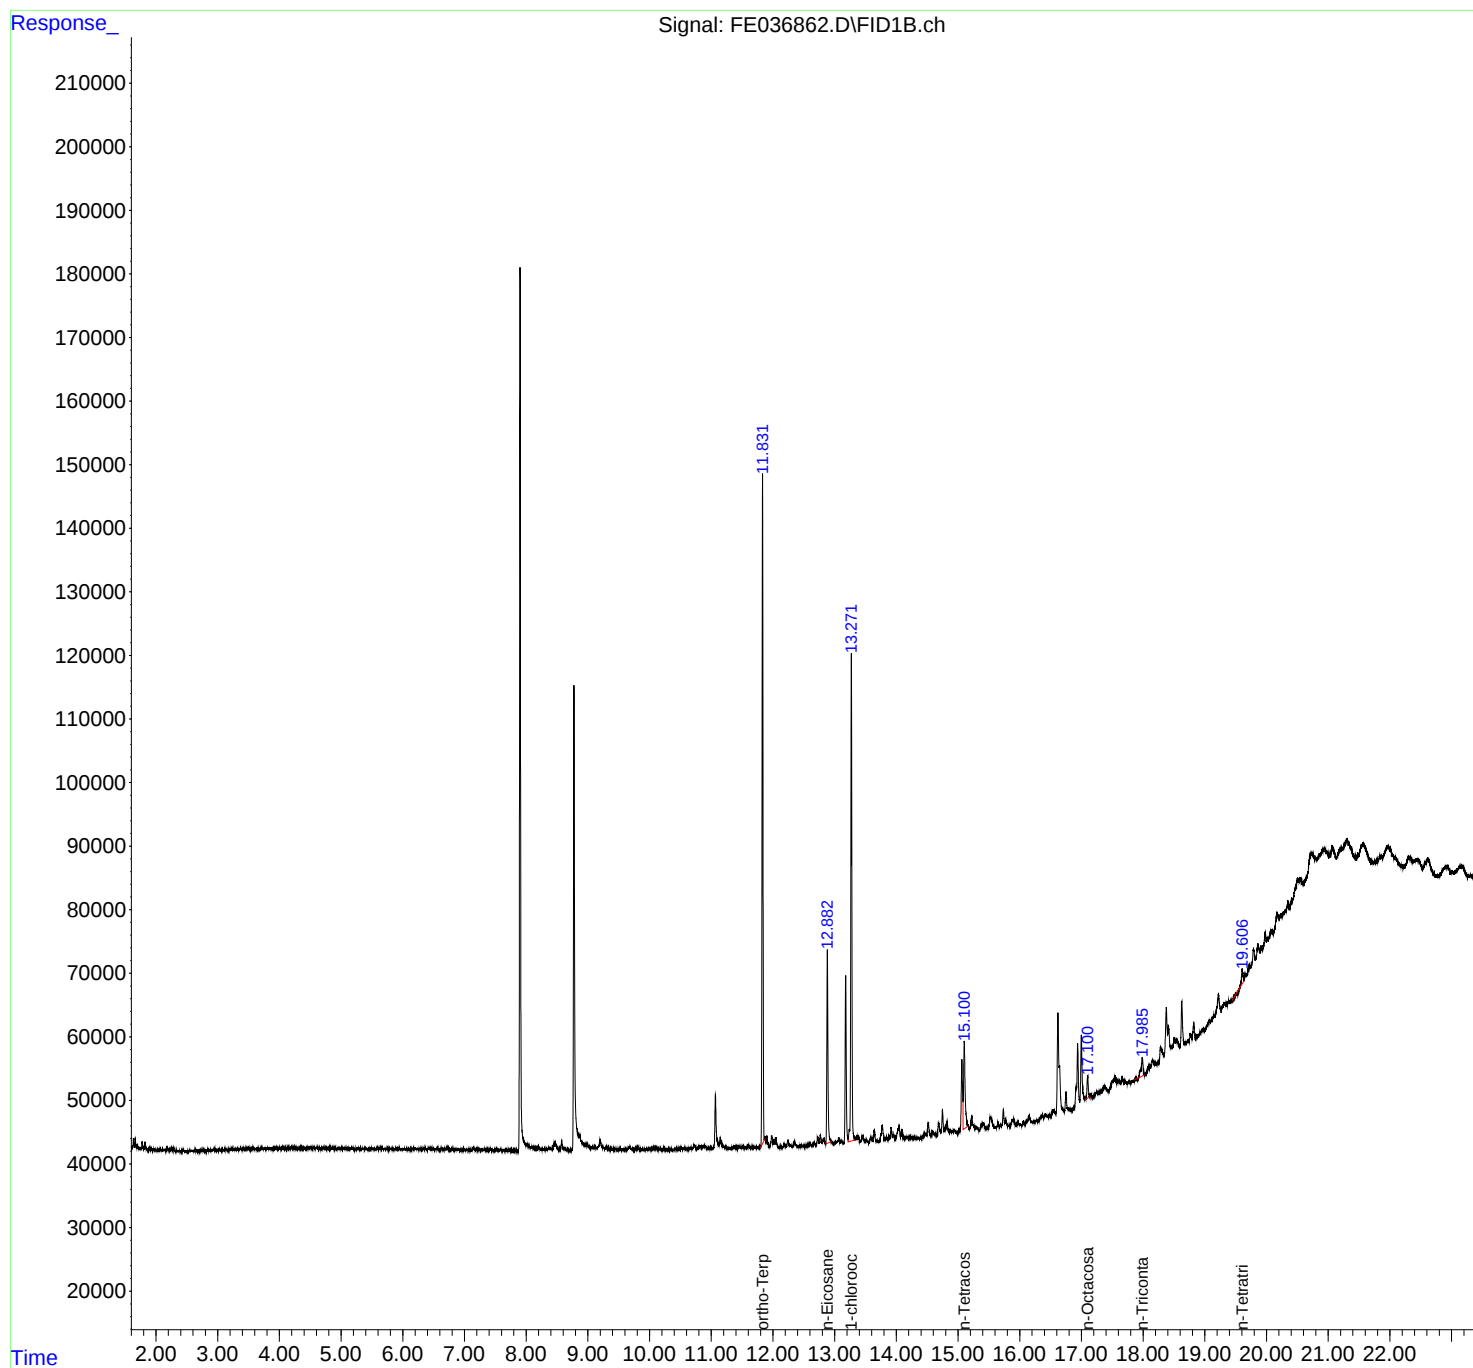


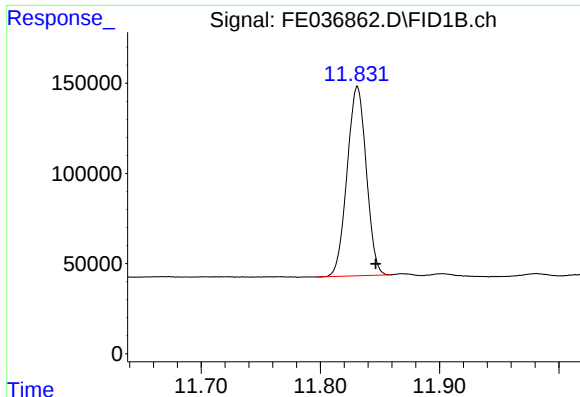

#9 ortho-Terphenyl (SURR)


R.T.: 11.831 min
Delta R.T.: -0.015 min
Response: 1175296
Conc: 6.31 ug/ml

Instrument :
FID_E
ClientSampleId :

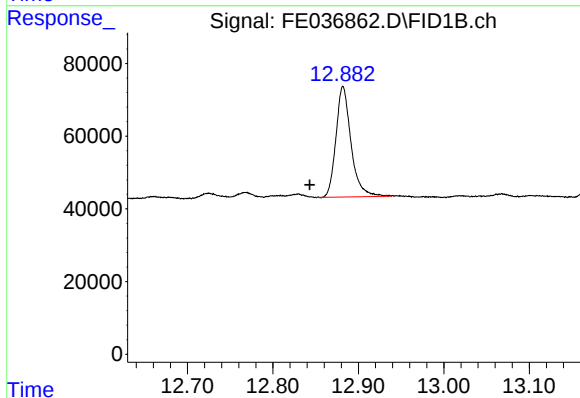


#10 n-Eicosane (C20)

R.T.: 12.882 min
Delta R.T.: 0.039 min
Response: 373089
Conc: 2.19 ug/ml

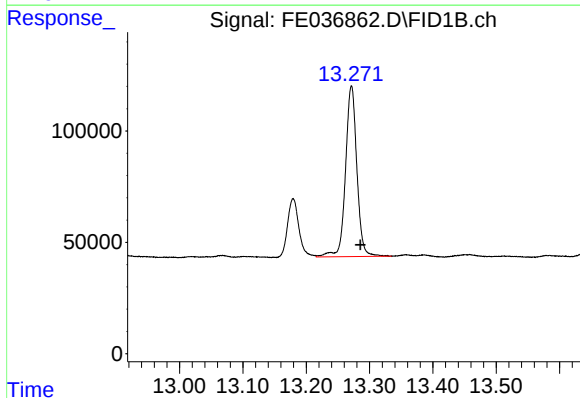


#12 1-chlorooctadecane (SURR)

R.T.: 13.271 min
Delta R.T.: -0.014 min
Response: 954952
Conc: 6.28 ug/ml

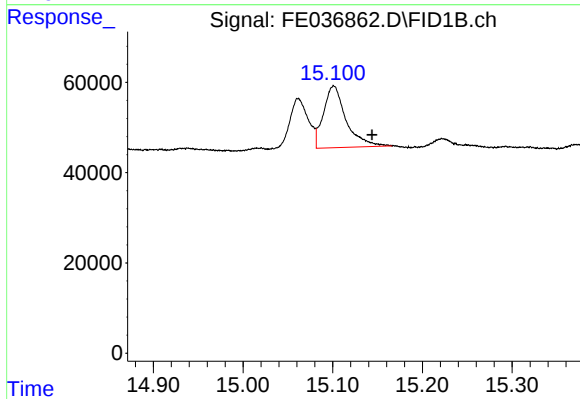

#14 n-Tetracosane (C24)


R.T.: 15.101 min
Delta R.T.: -0.043 min
Response: 239337
Conc: 1.40 ug/ml

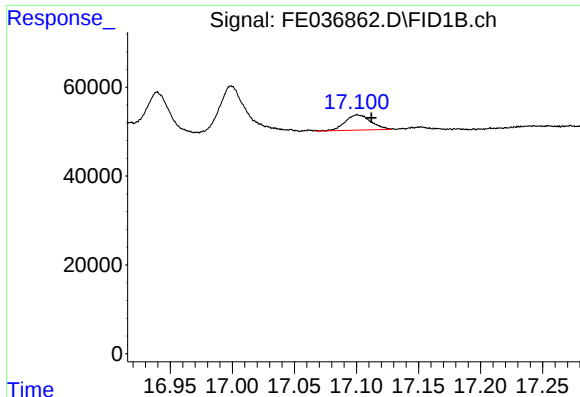

#16 n-Octacosane (C28)


R.T.: 17.101 min
Delta R.T.: -0.011 min
Response: 48536
Conc: 0.30 ug/ml

Instrument :
FID_E
ClientSampleId :

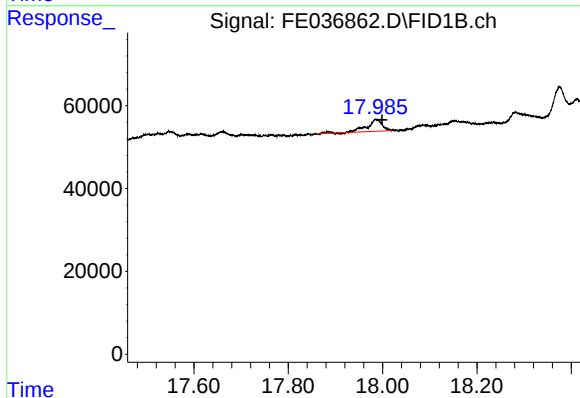

#17 n-Tricontane (C30)

R.T.: 17.985 min
Delta R.T.: -0.013 min
Response: 63932
Conc: 0.42 ug/ml

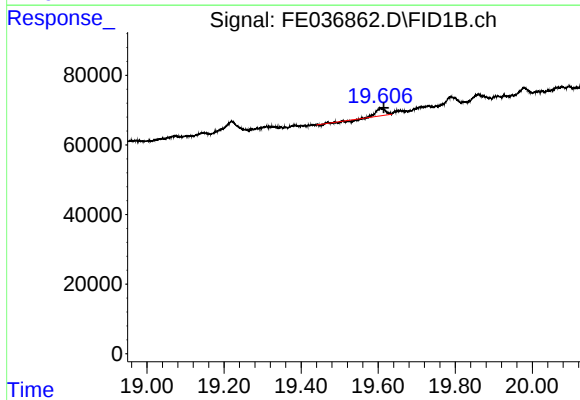

#19 n-Tetratriacontane (C34)

R.T.: 19.606 min
Delta R.T.: -0.009 min
Response: 26947
Conc: 0.32 ug/ml