

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080524\
Data File : FE049445.D
Signal(s) : FID1B.ch
Acq On : 05 Aug 2024 11:05
Operator : YP\AJ
Sample : PB162389BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 06 01:11:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072924.M
Quant Title :
QLast Update : Tue Jul 30 04:50:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.981	2372596	18.554 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.870	48382	0.344 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080524\
Data File : FE049445.D
Signal(s) : FID1B.ch
Acq On : 05 Aug 2024 11:05
Operator : YP\AJ
Sample : PB162389BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Aug 06 01:11:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072924.M
Quant Title :
QLast Update : Tue Jul 30 04:50:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

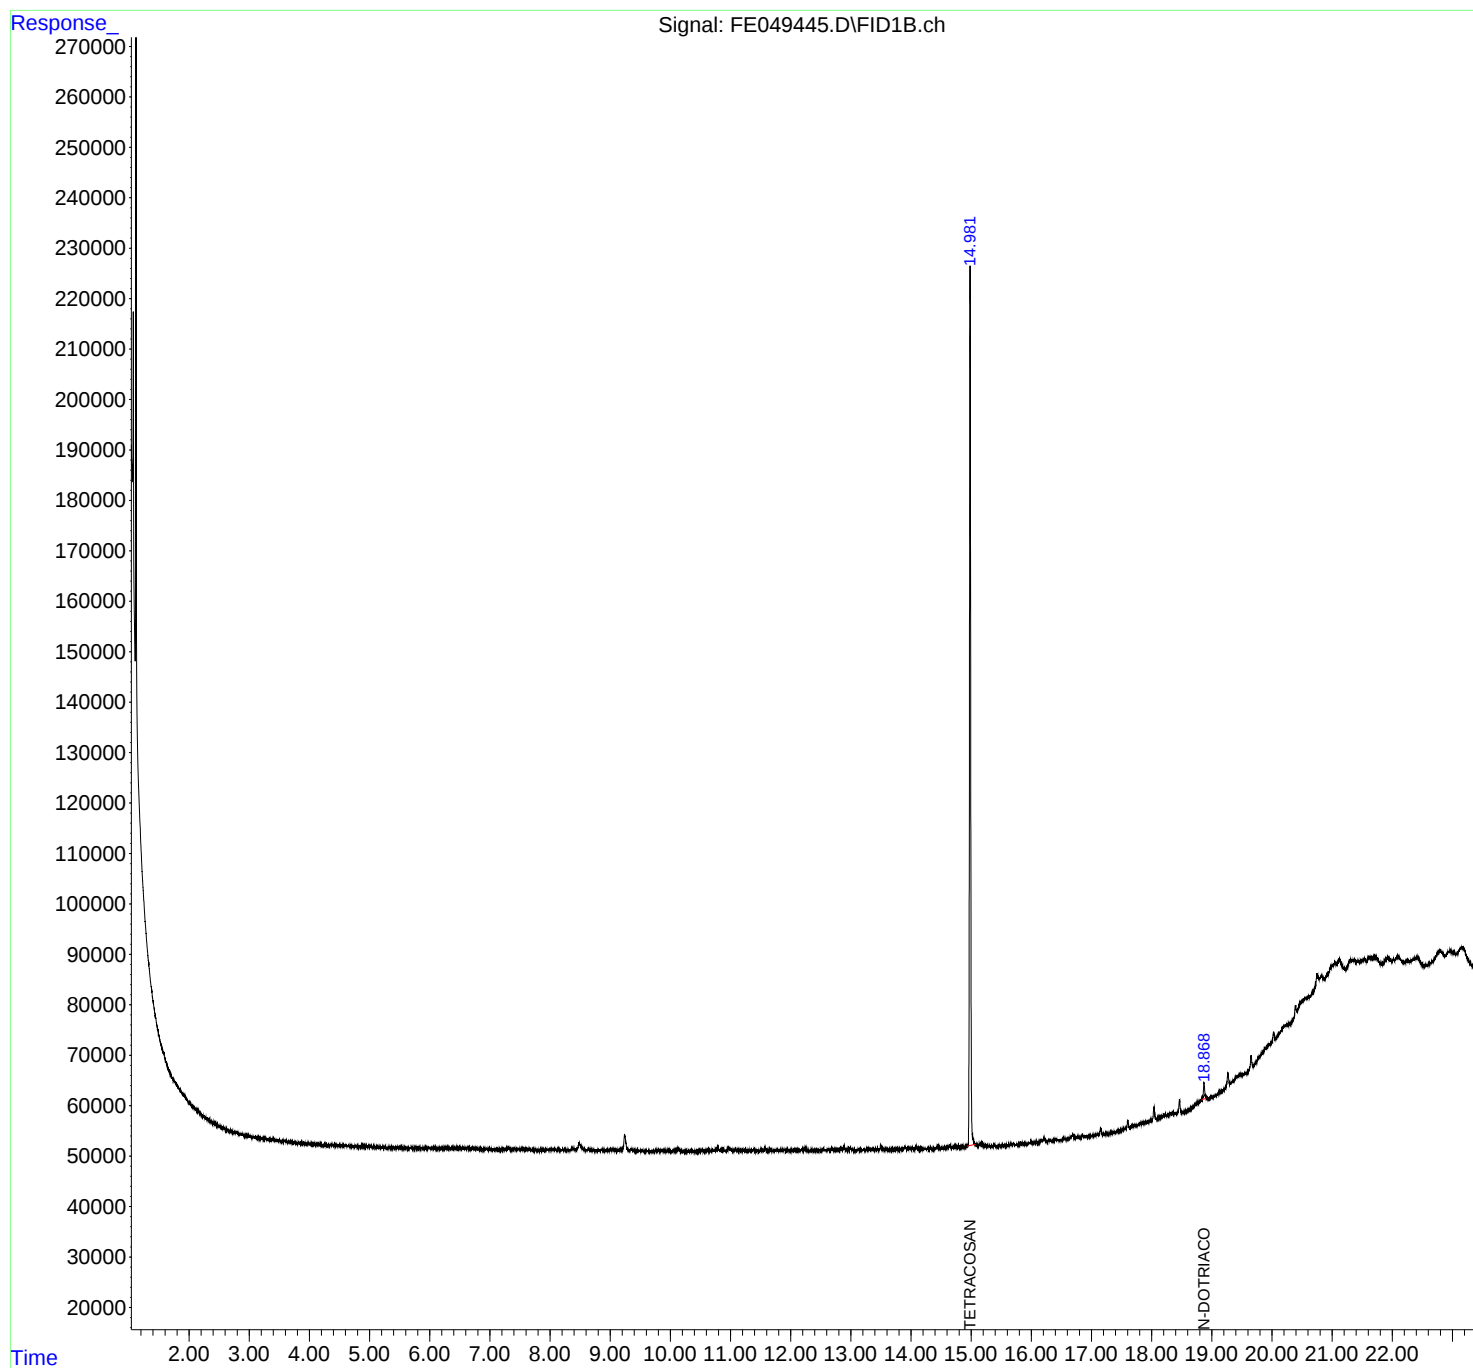


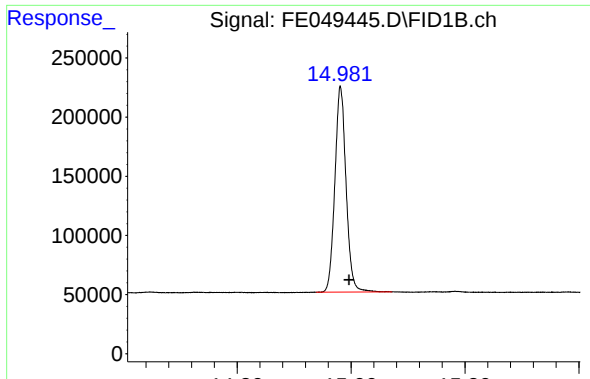

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.981 min
Delta R.T.: -0.015 min
Response: 2372596
Conc: 18.55 ug/ml

Instrument :
FID_E
ClientSampleId :

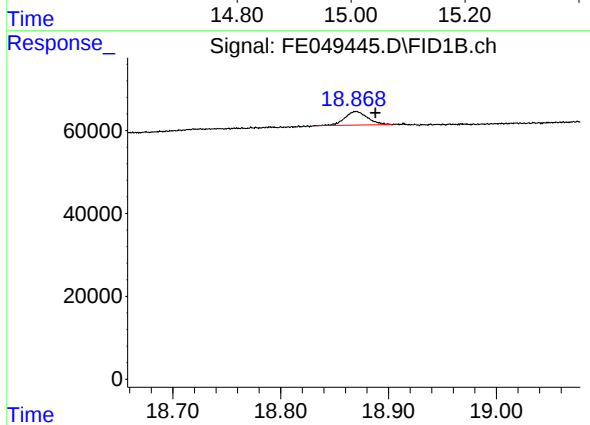

#14 N-DOTRIACONTANE

R.T.: 18.870 min
Delta R.T.: -0.018 min
Response: 48382
Conc: 0.34 ug/ml