

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080524\
Data File : FE049450.D
Signal(s) : FID1B.ch
Acq On : 05 Aug 2024 14:42
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 98 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 06 01:12:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072924.M
Quant Title :
QLast Update : Tue Jul 30 04:50:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.982	2470884	19.322 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE080524\
Data File : FE049450.D
Signal(s) : FID1B.ch
Acq On : 05 Aug 2024 14:42
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 98 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Aug 06 01:12:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE072924.M
Quant Title :
QLast Update : Tue Jul 30 04:50:04 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

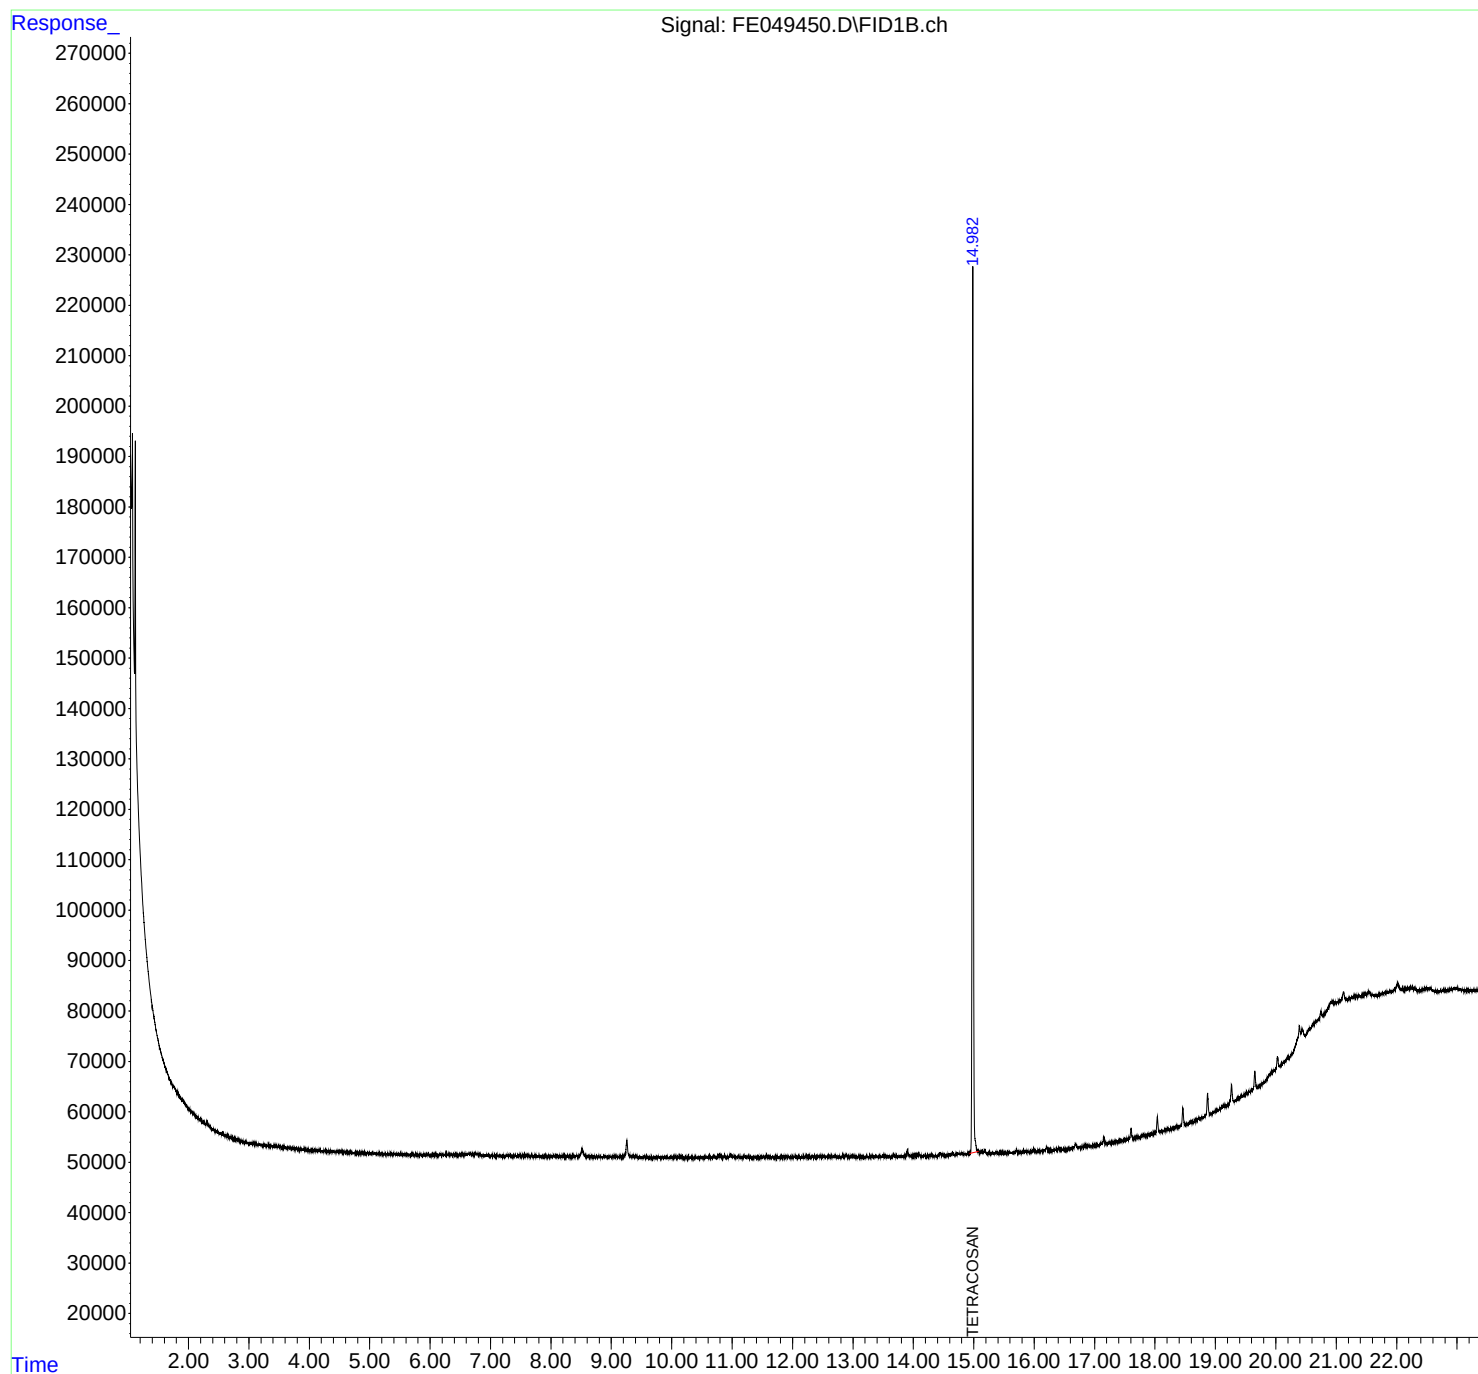

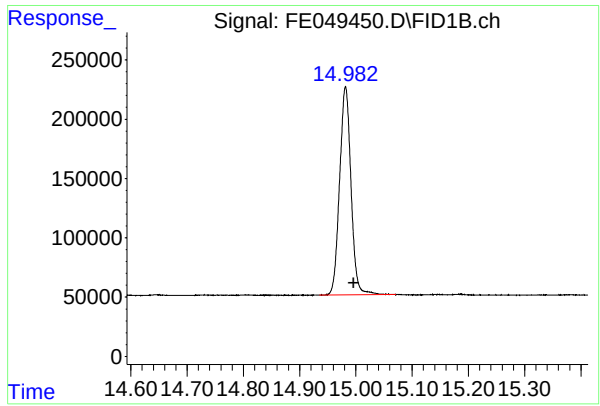

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.982 min
Delta R.T.: -0.015 min
Response: 2470884
Conc: 19.32 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK